




Wind Speed

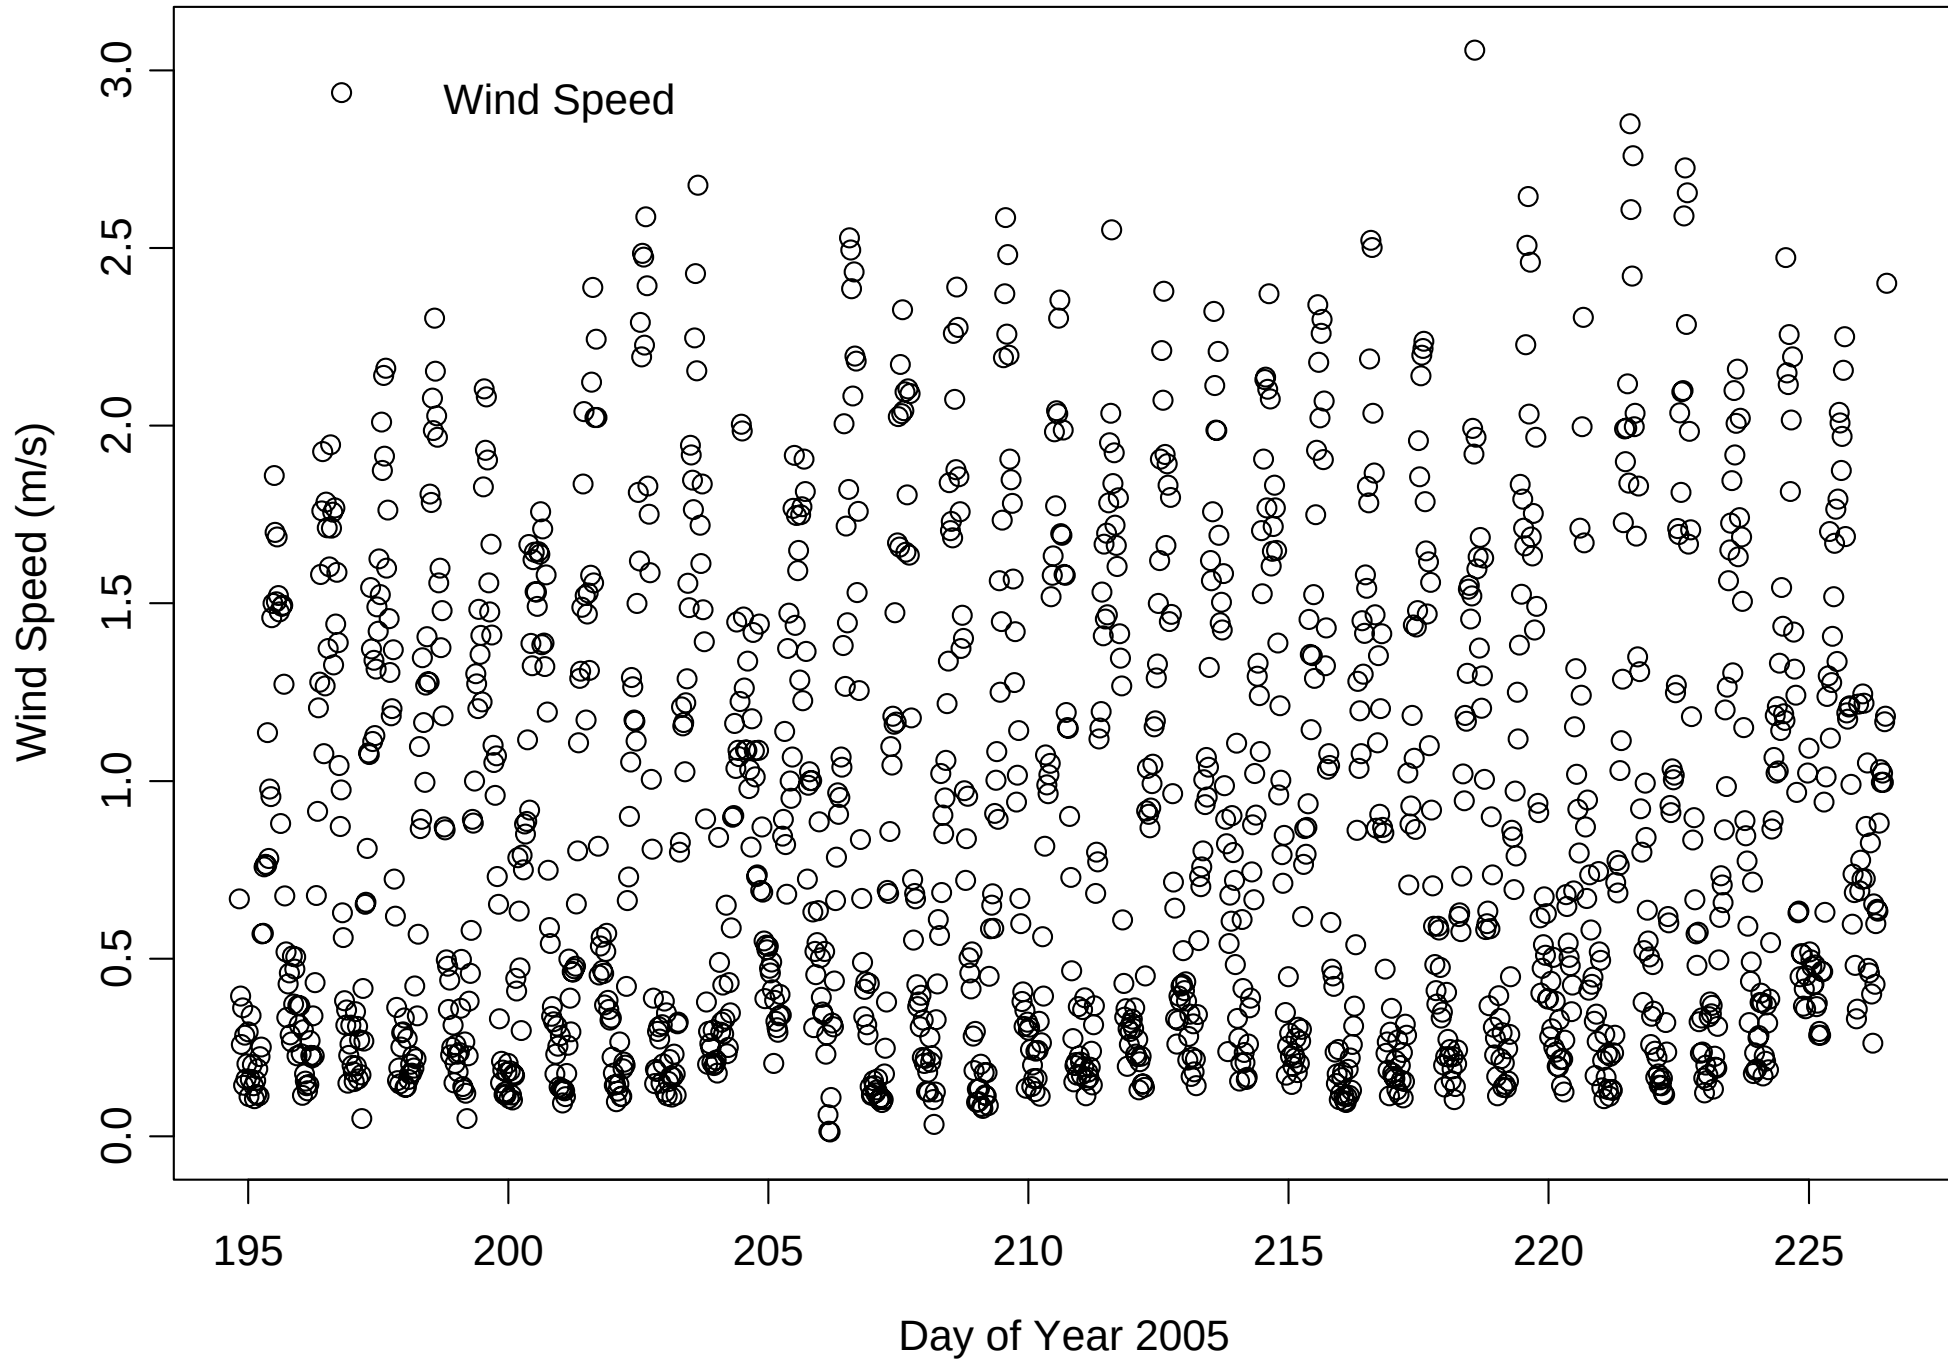


Wind Direction

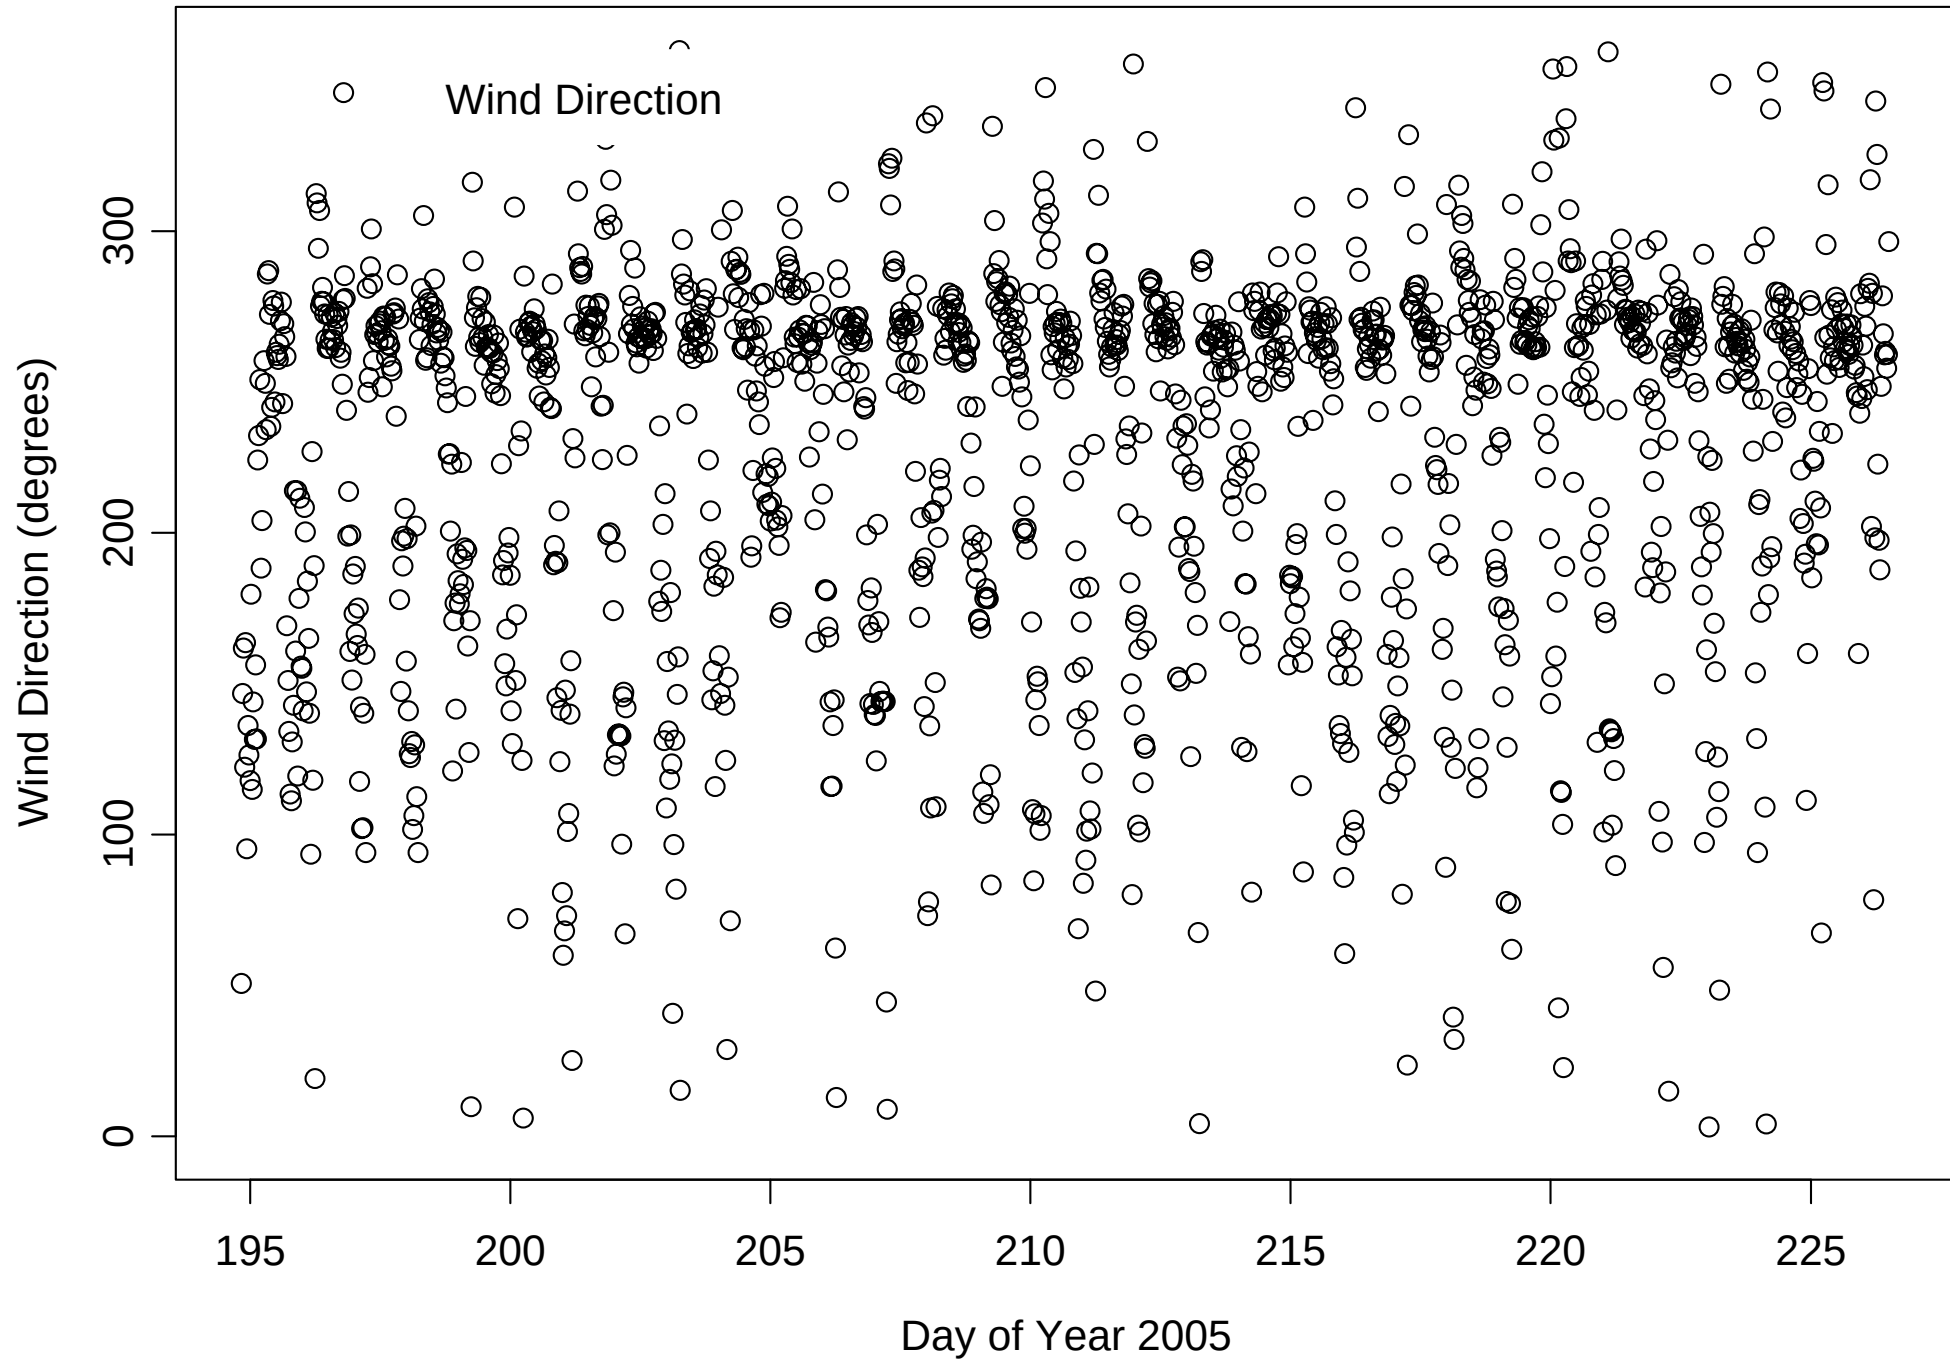


Ozone Concentration

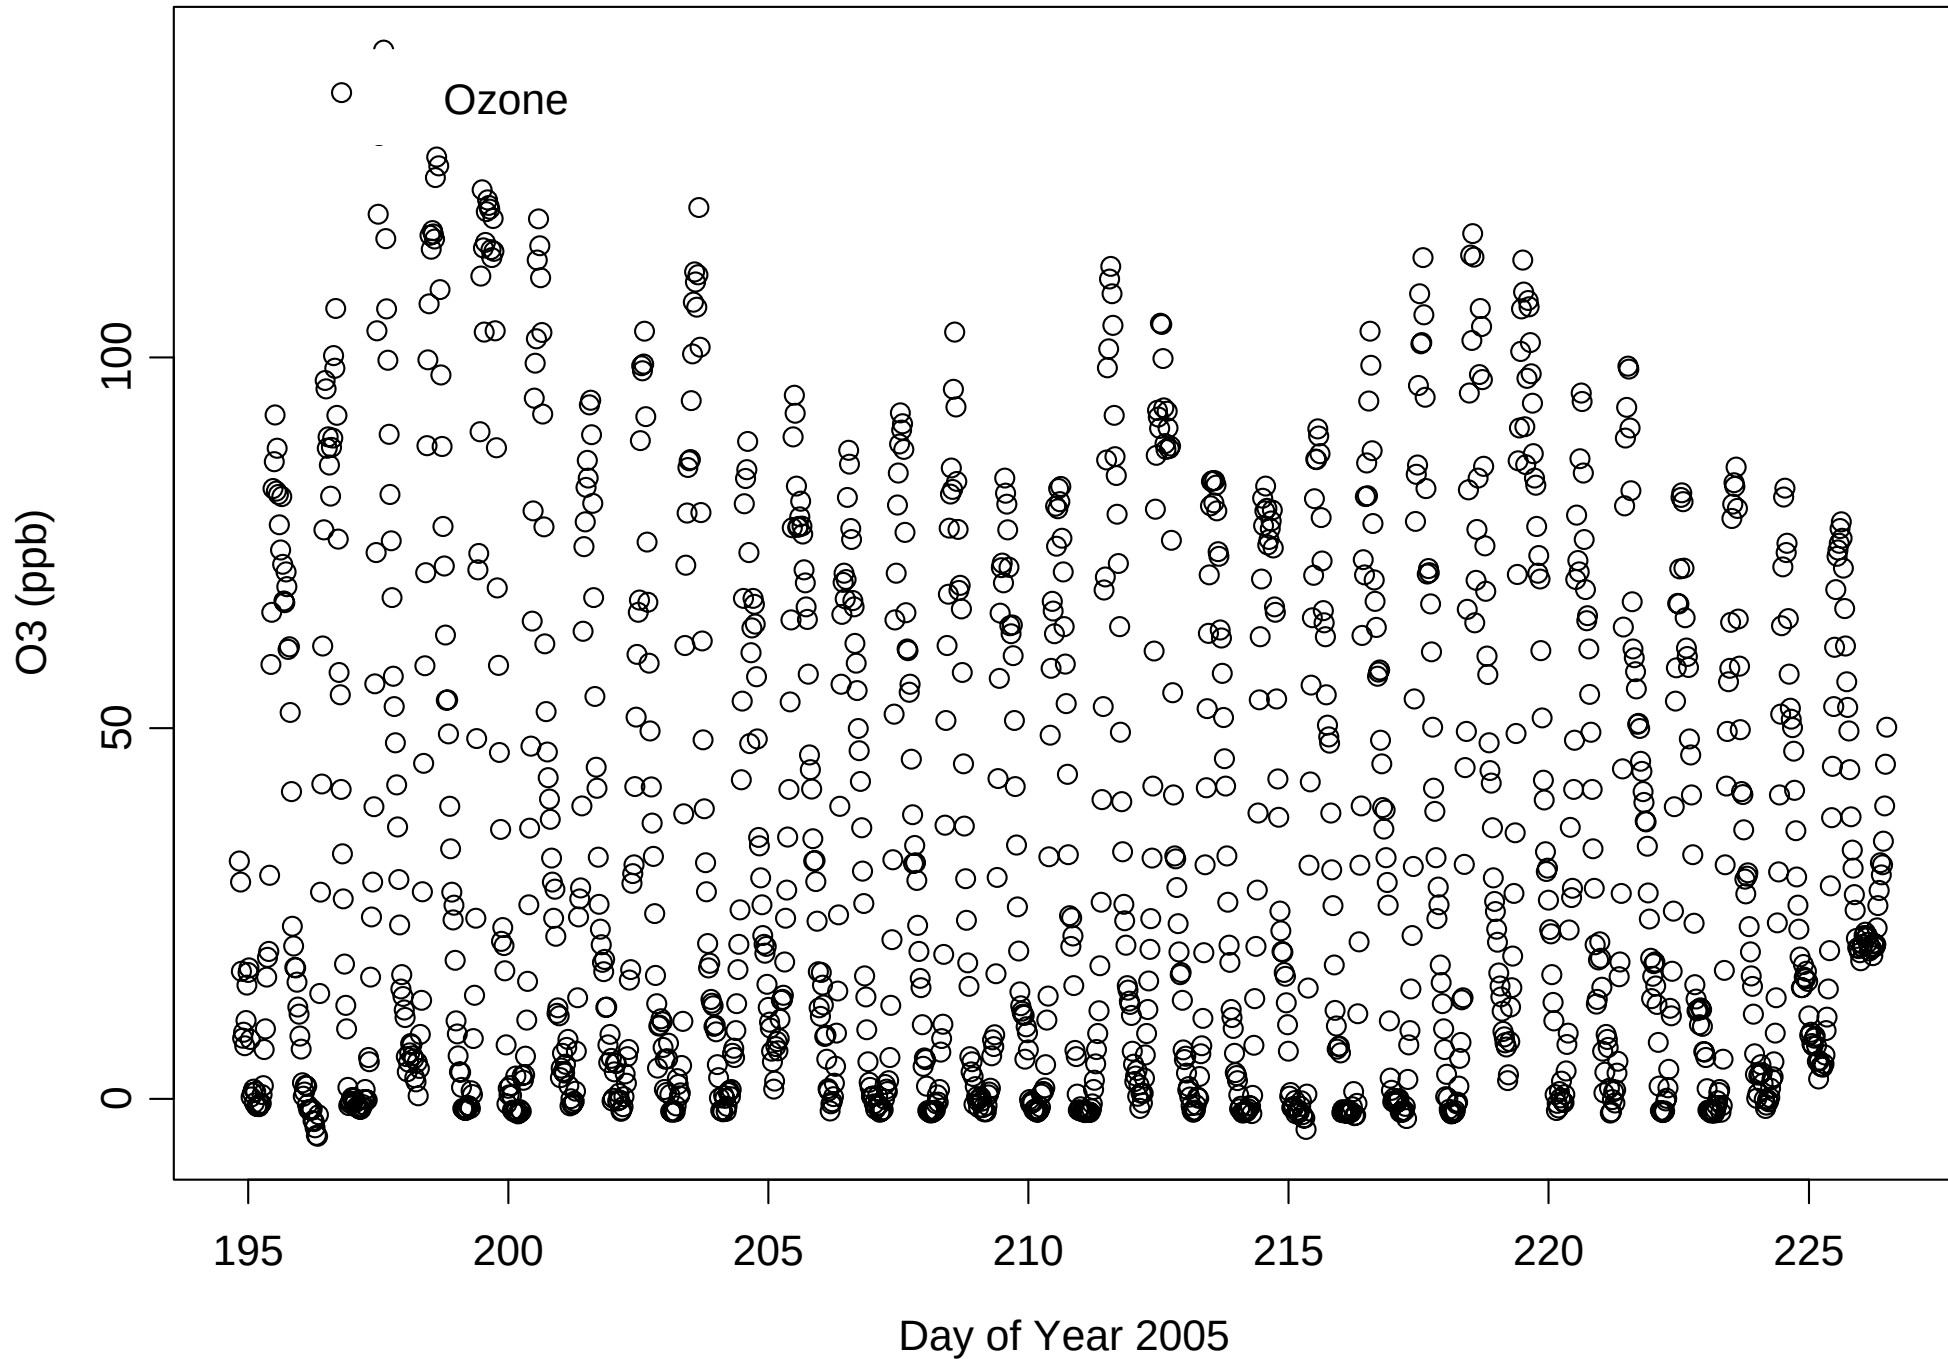


PAR

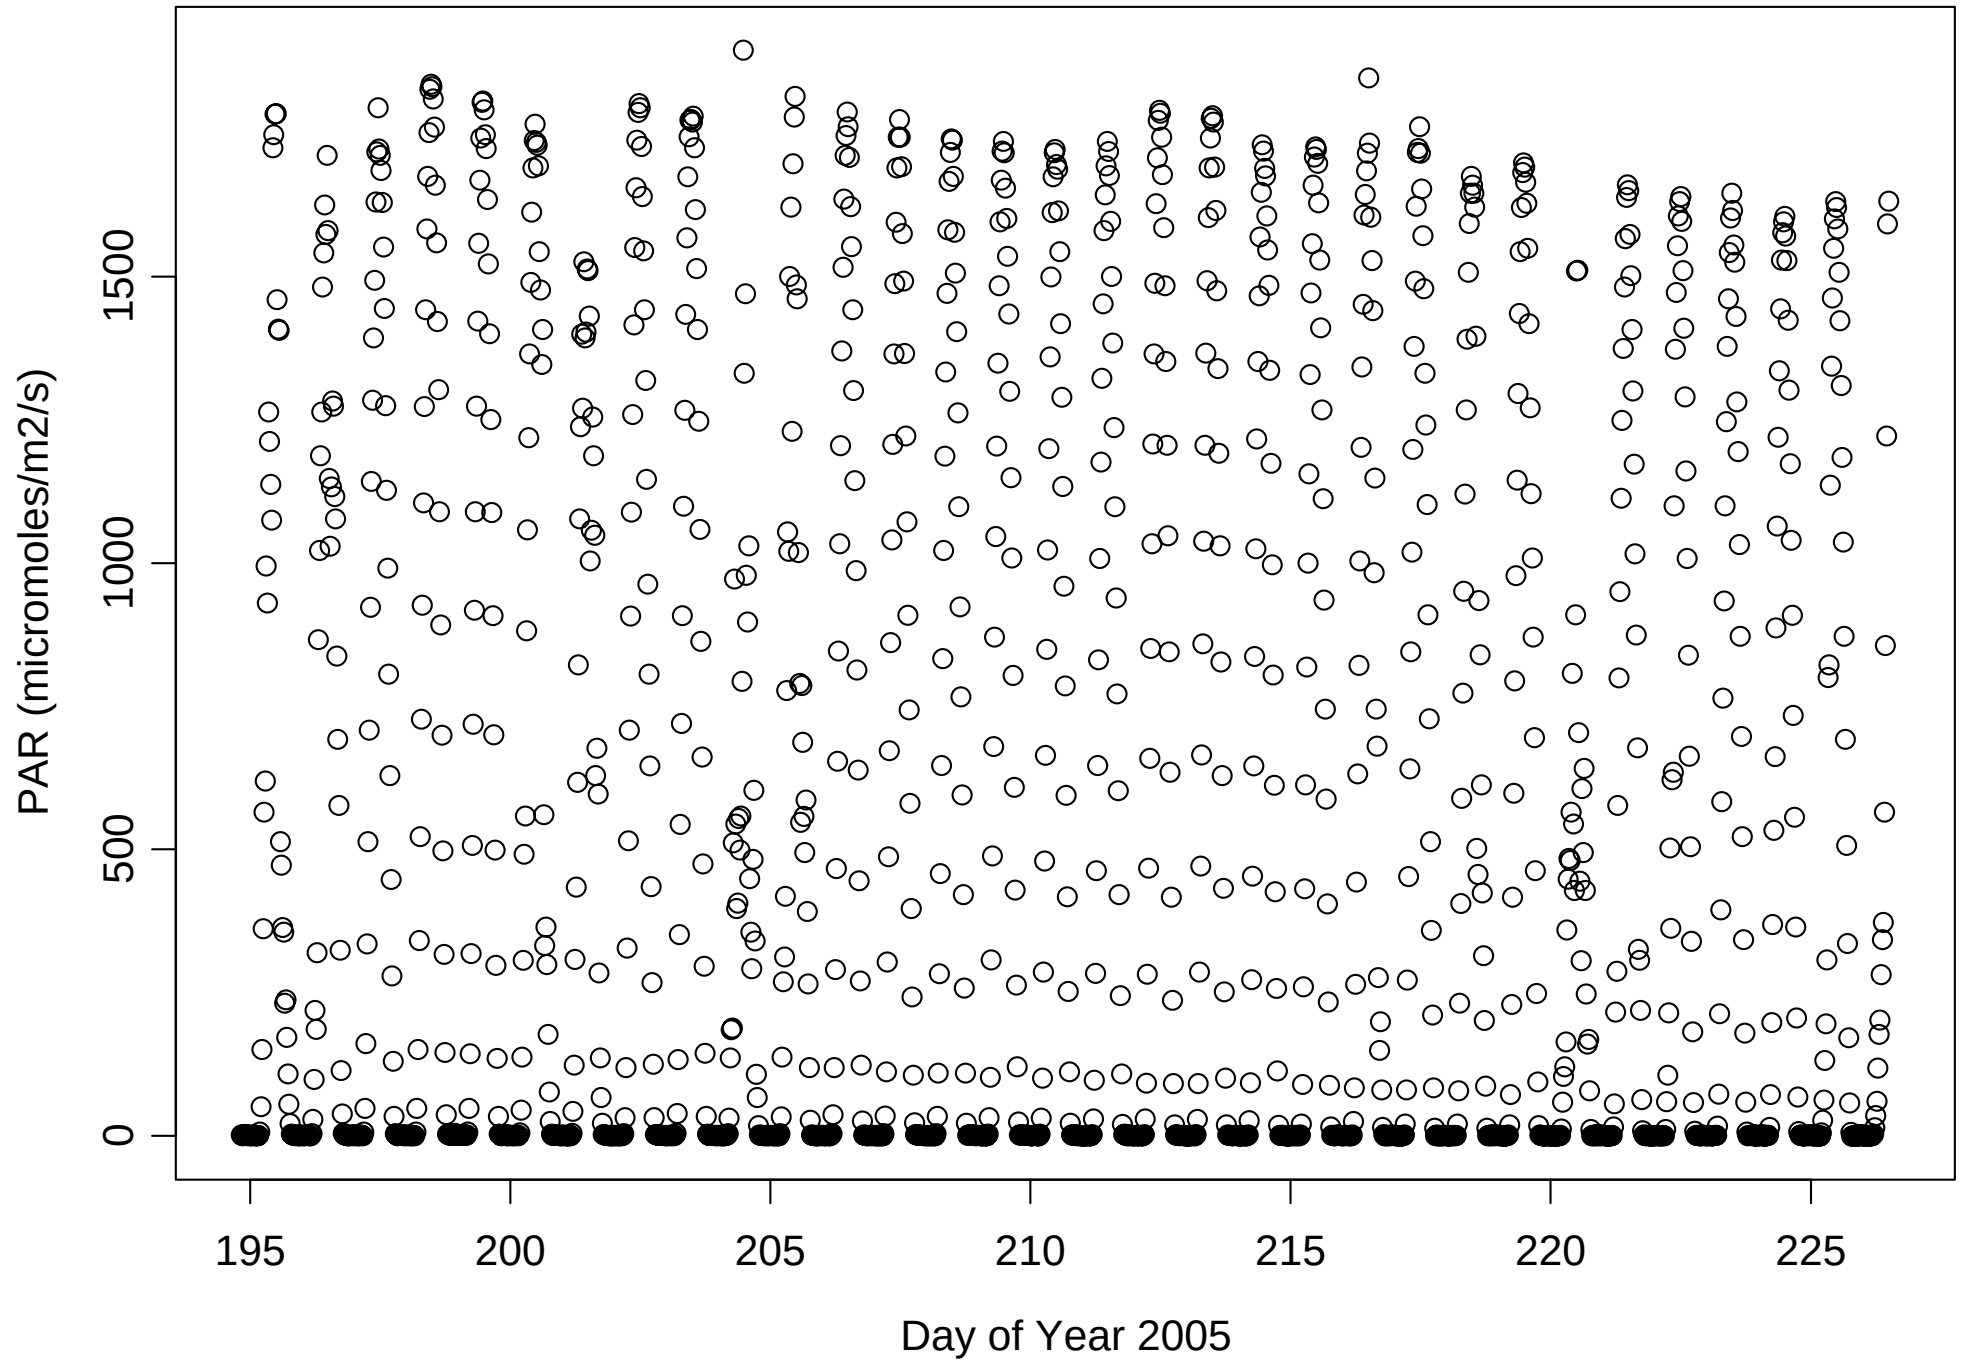


Relative Humidity

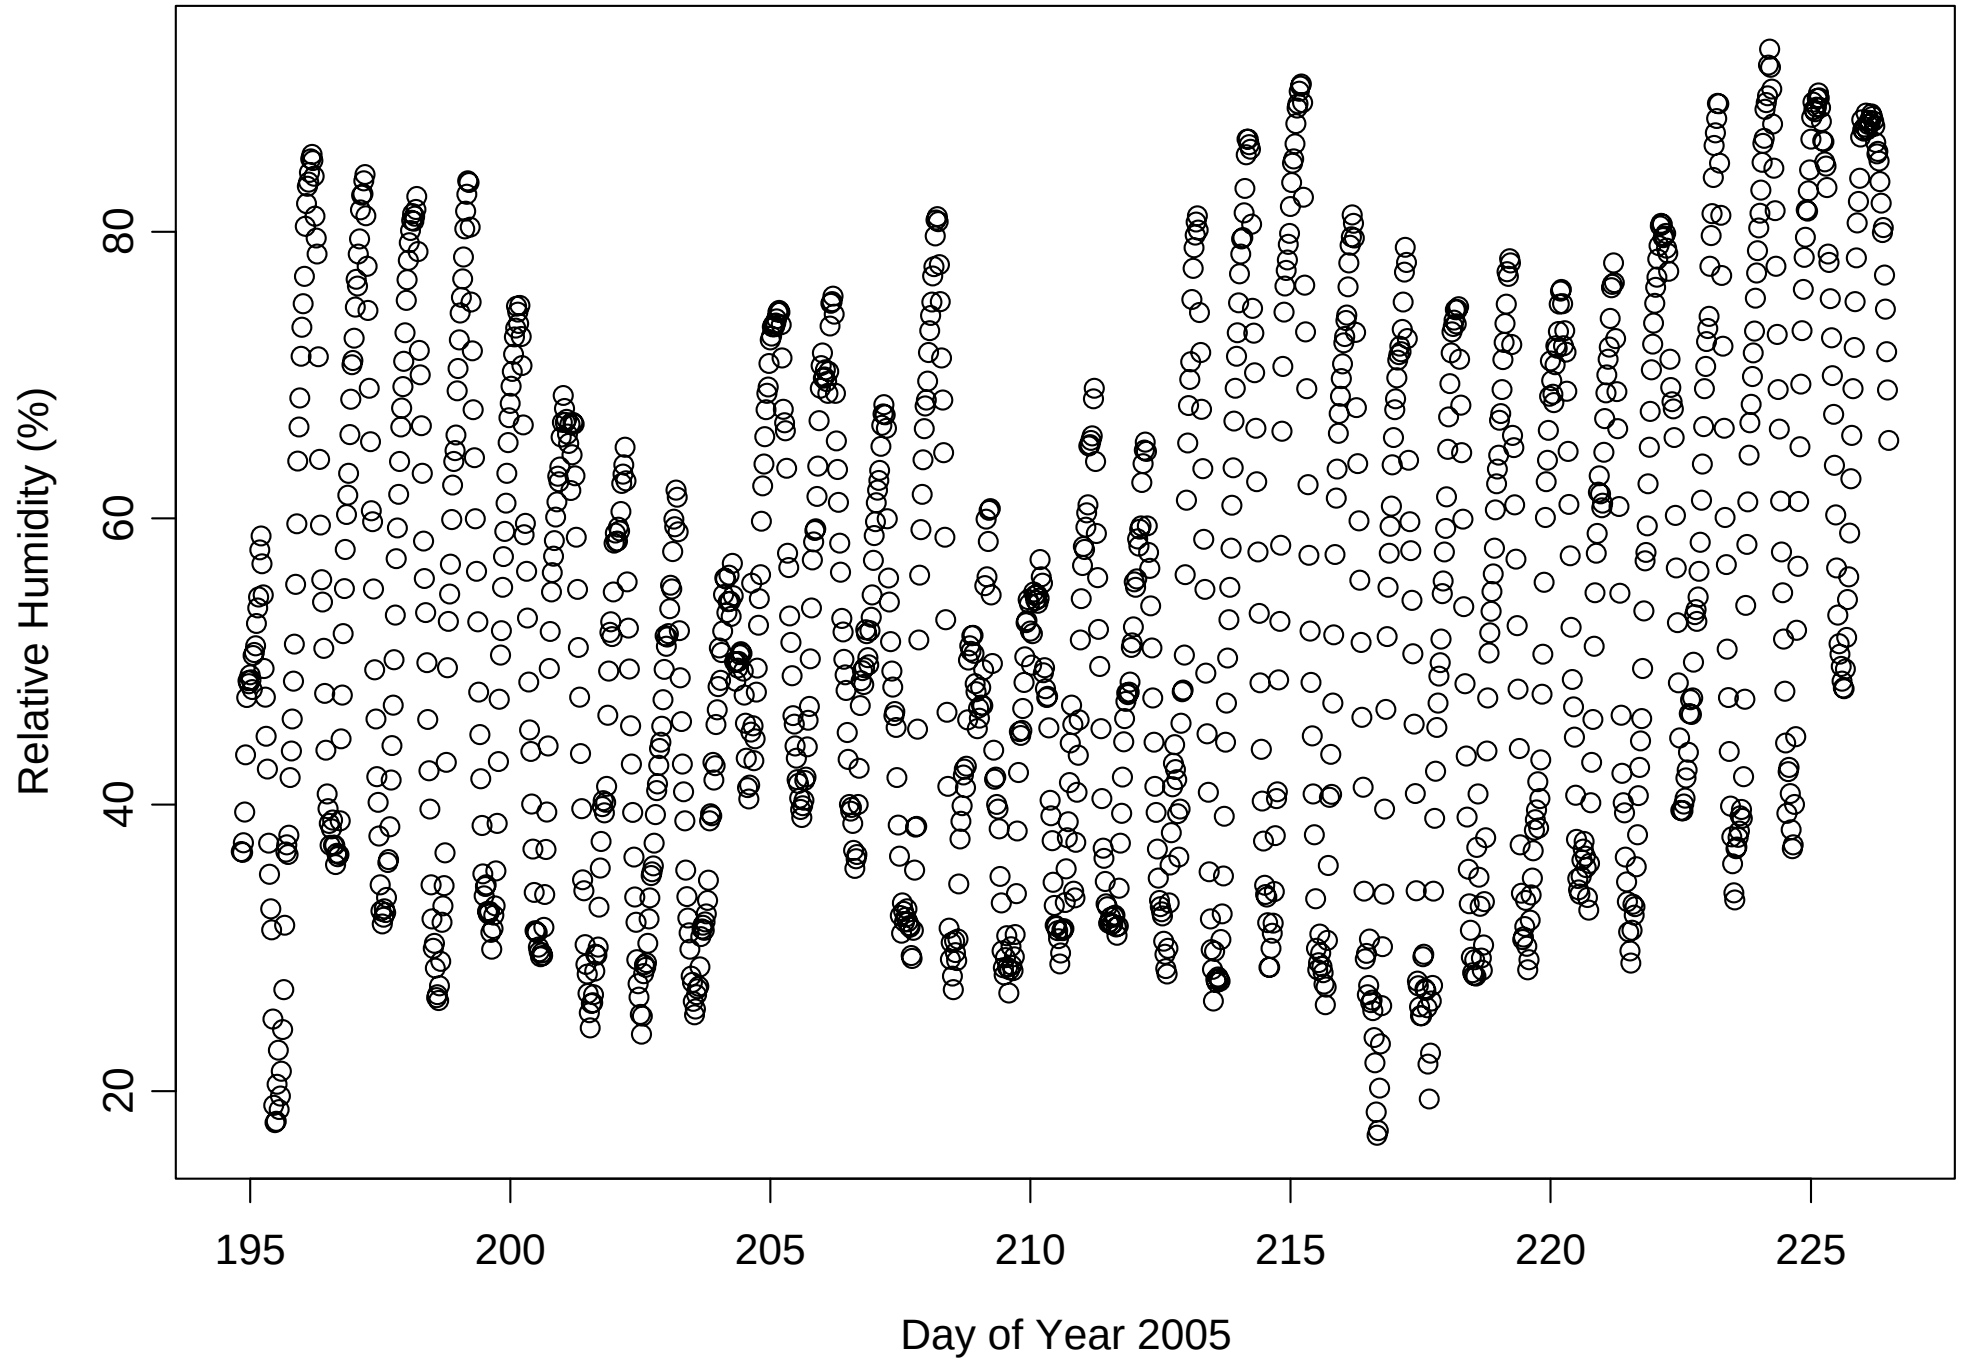


Room and Air Temperature

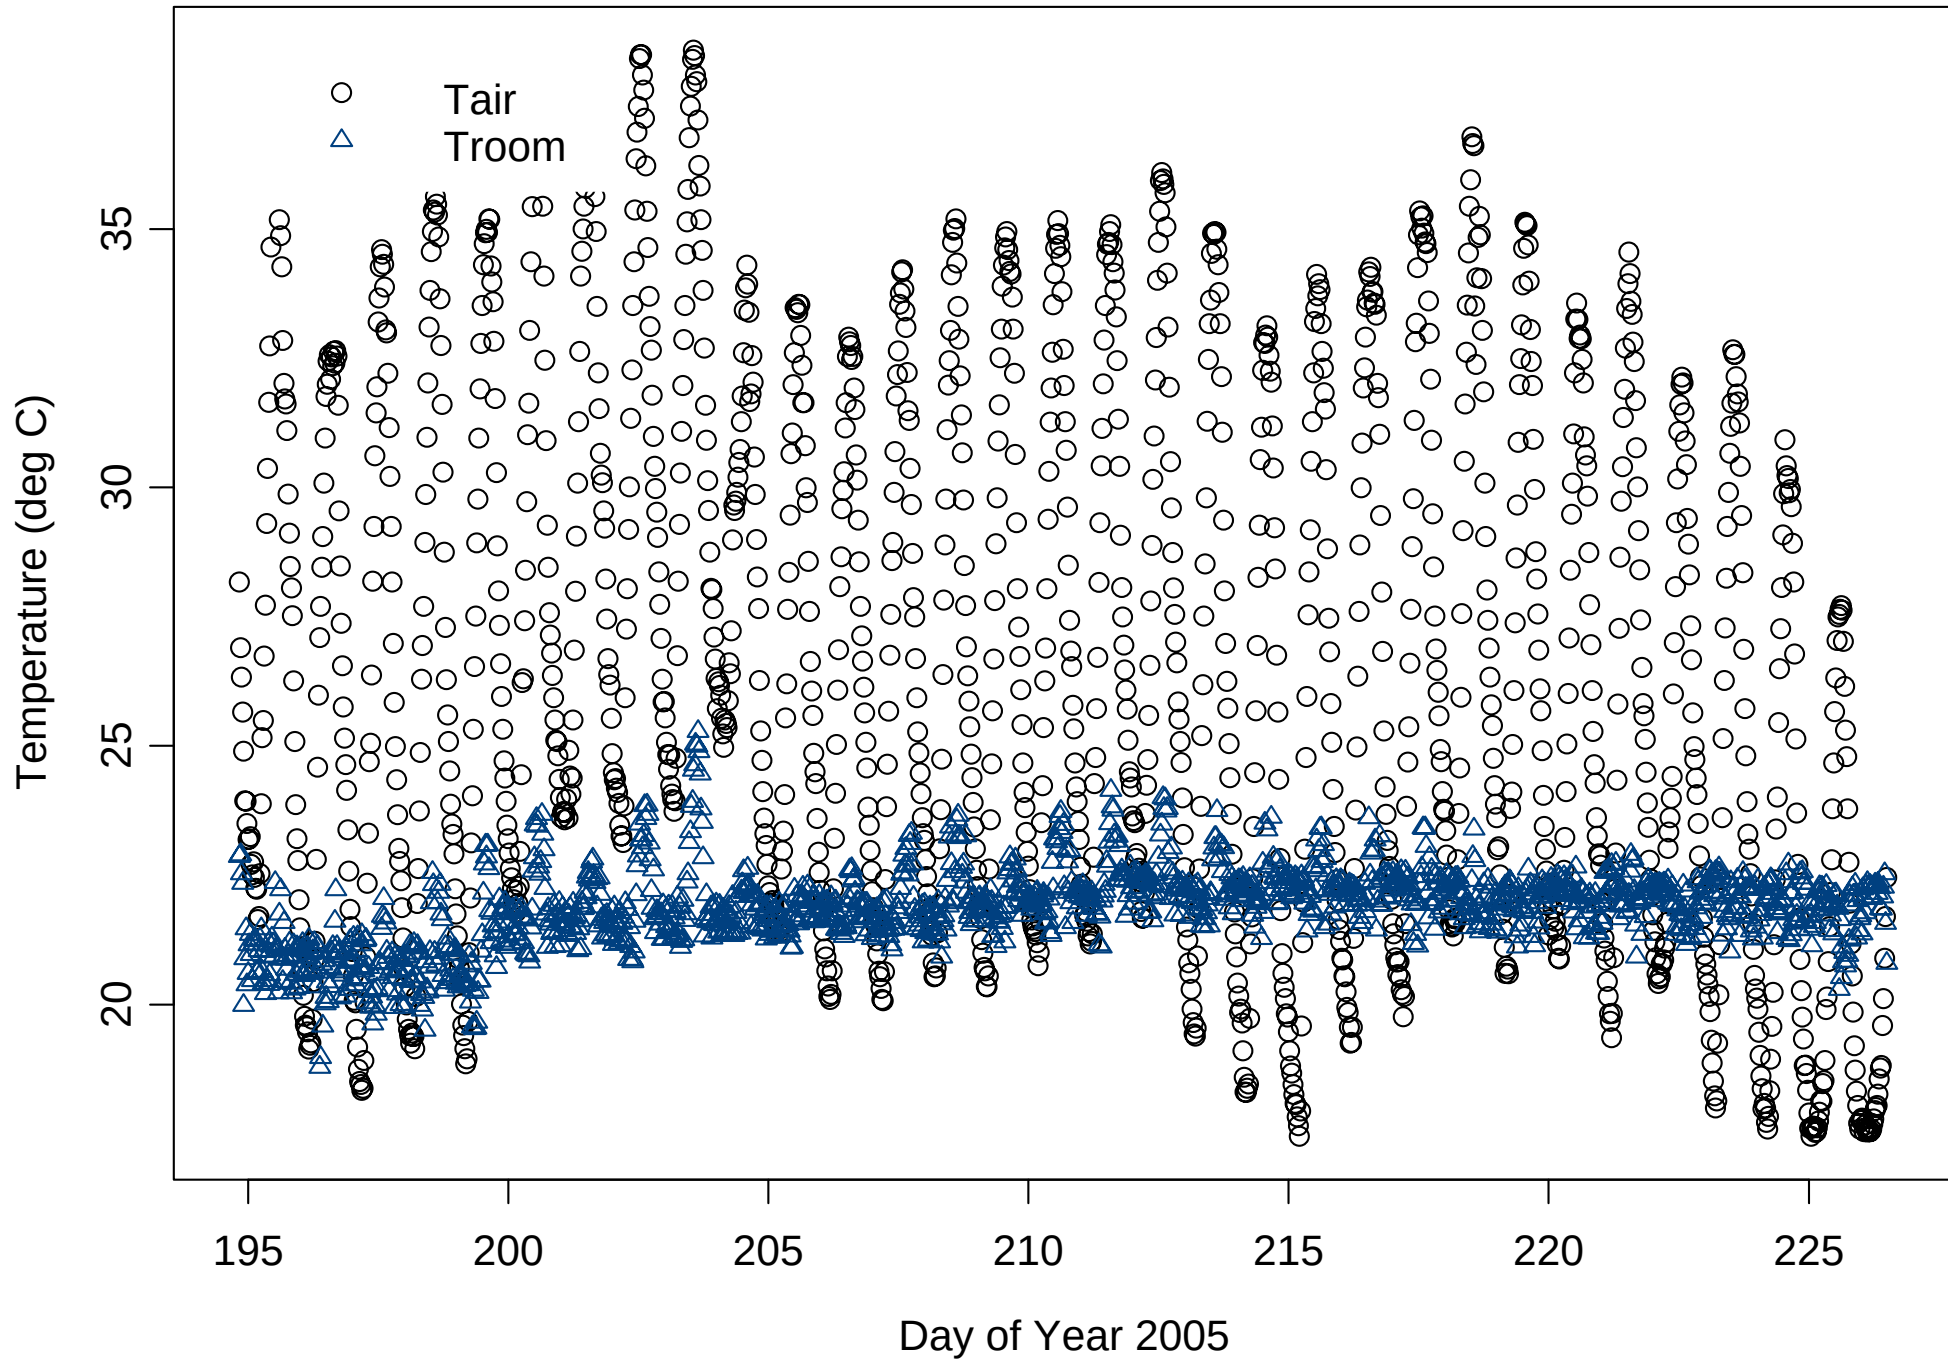


Rainfall

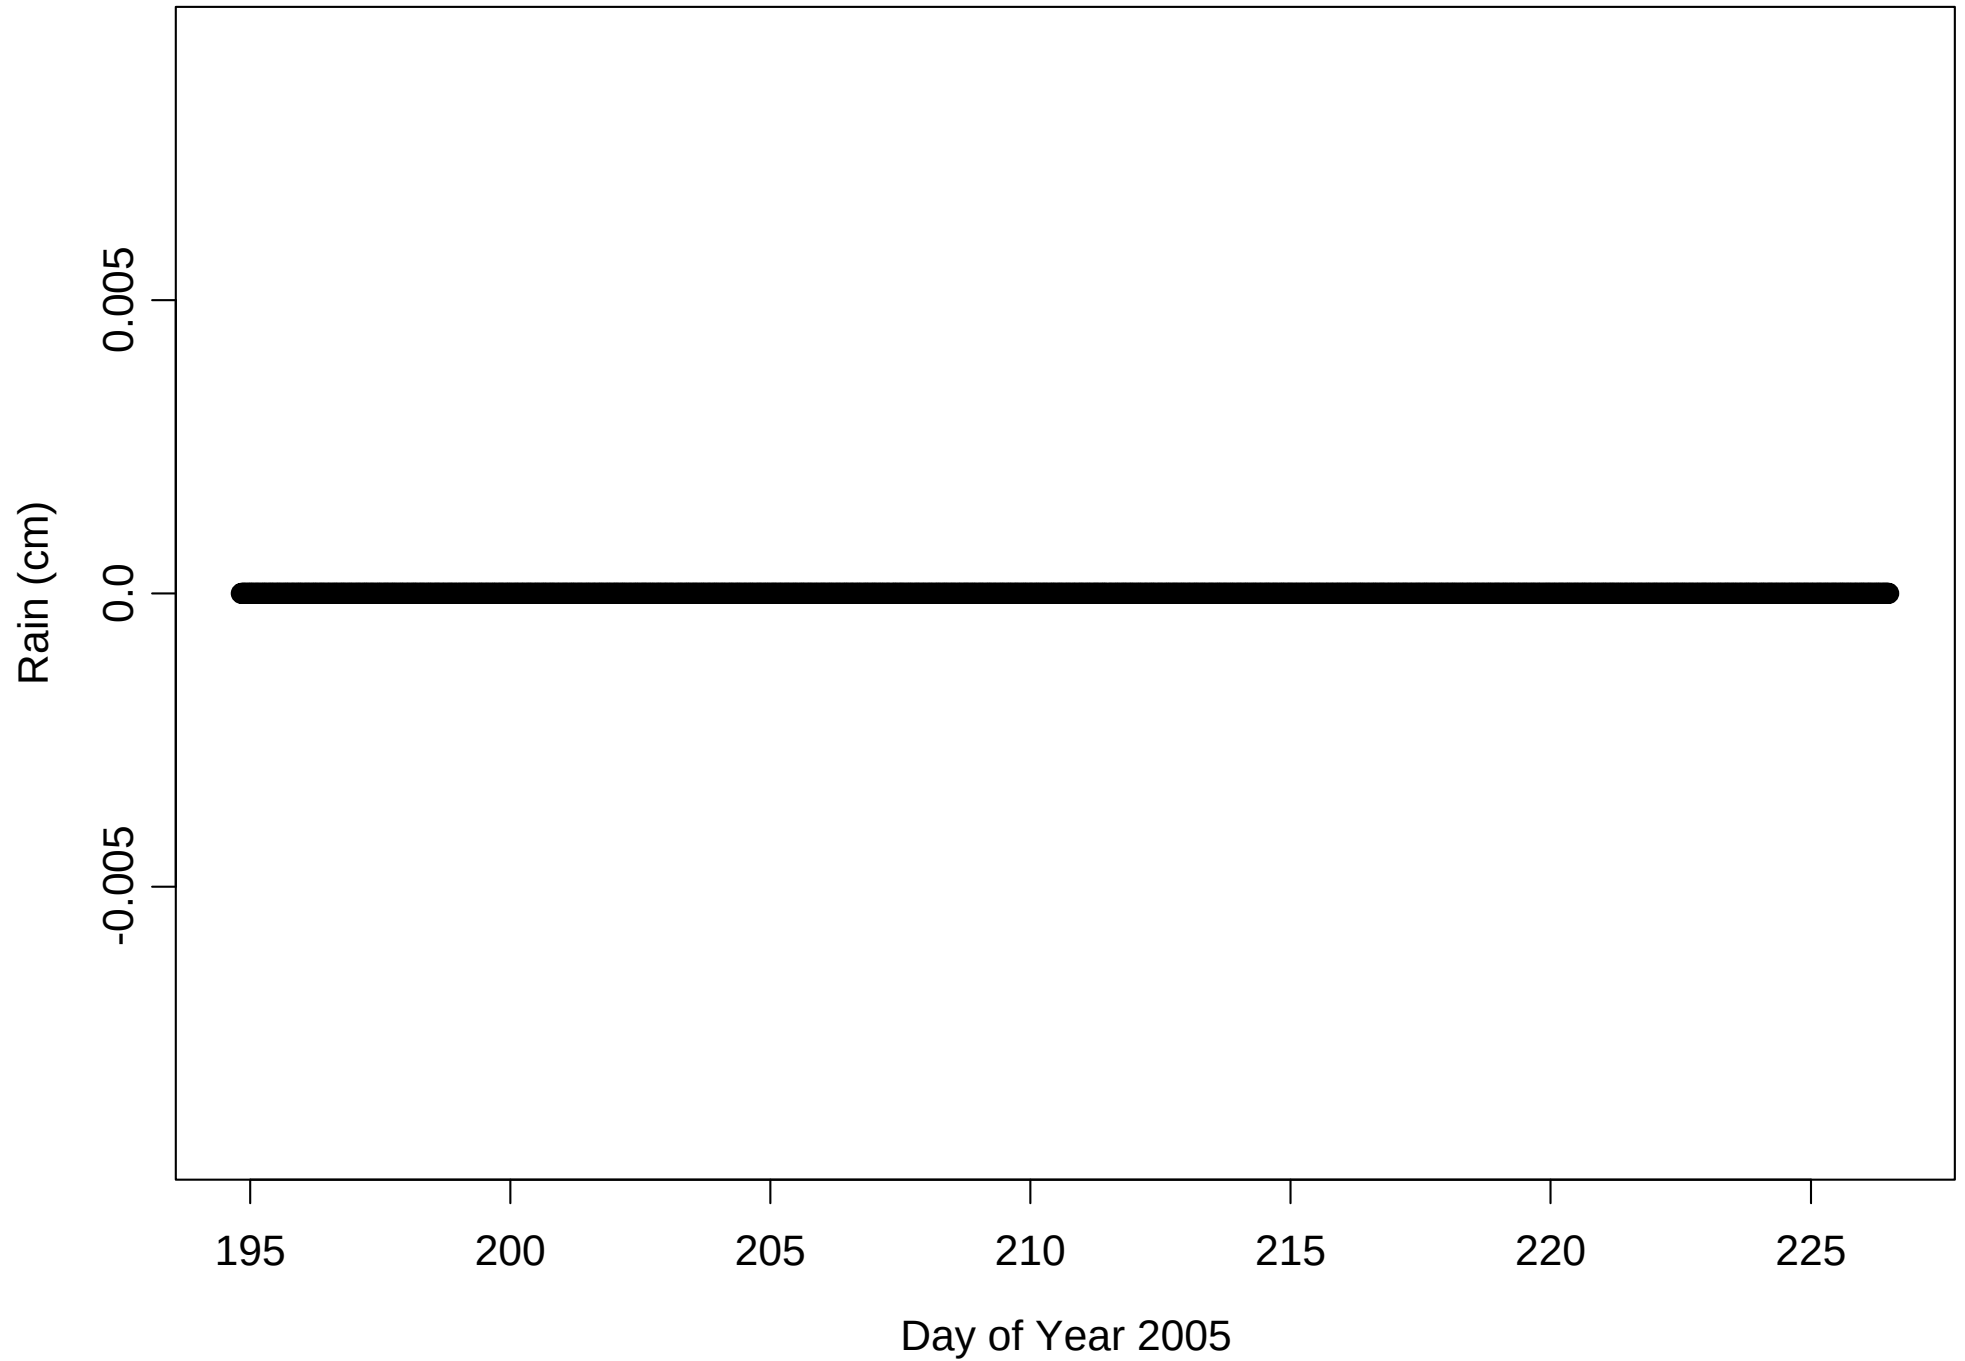


Atmospheric Pressure

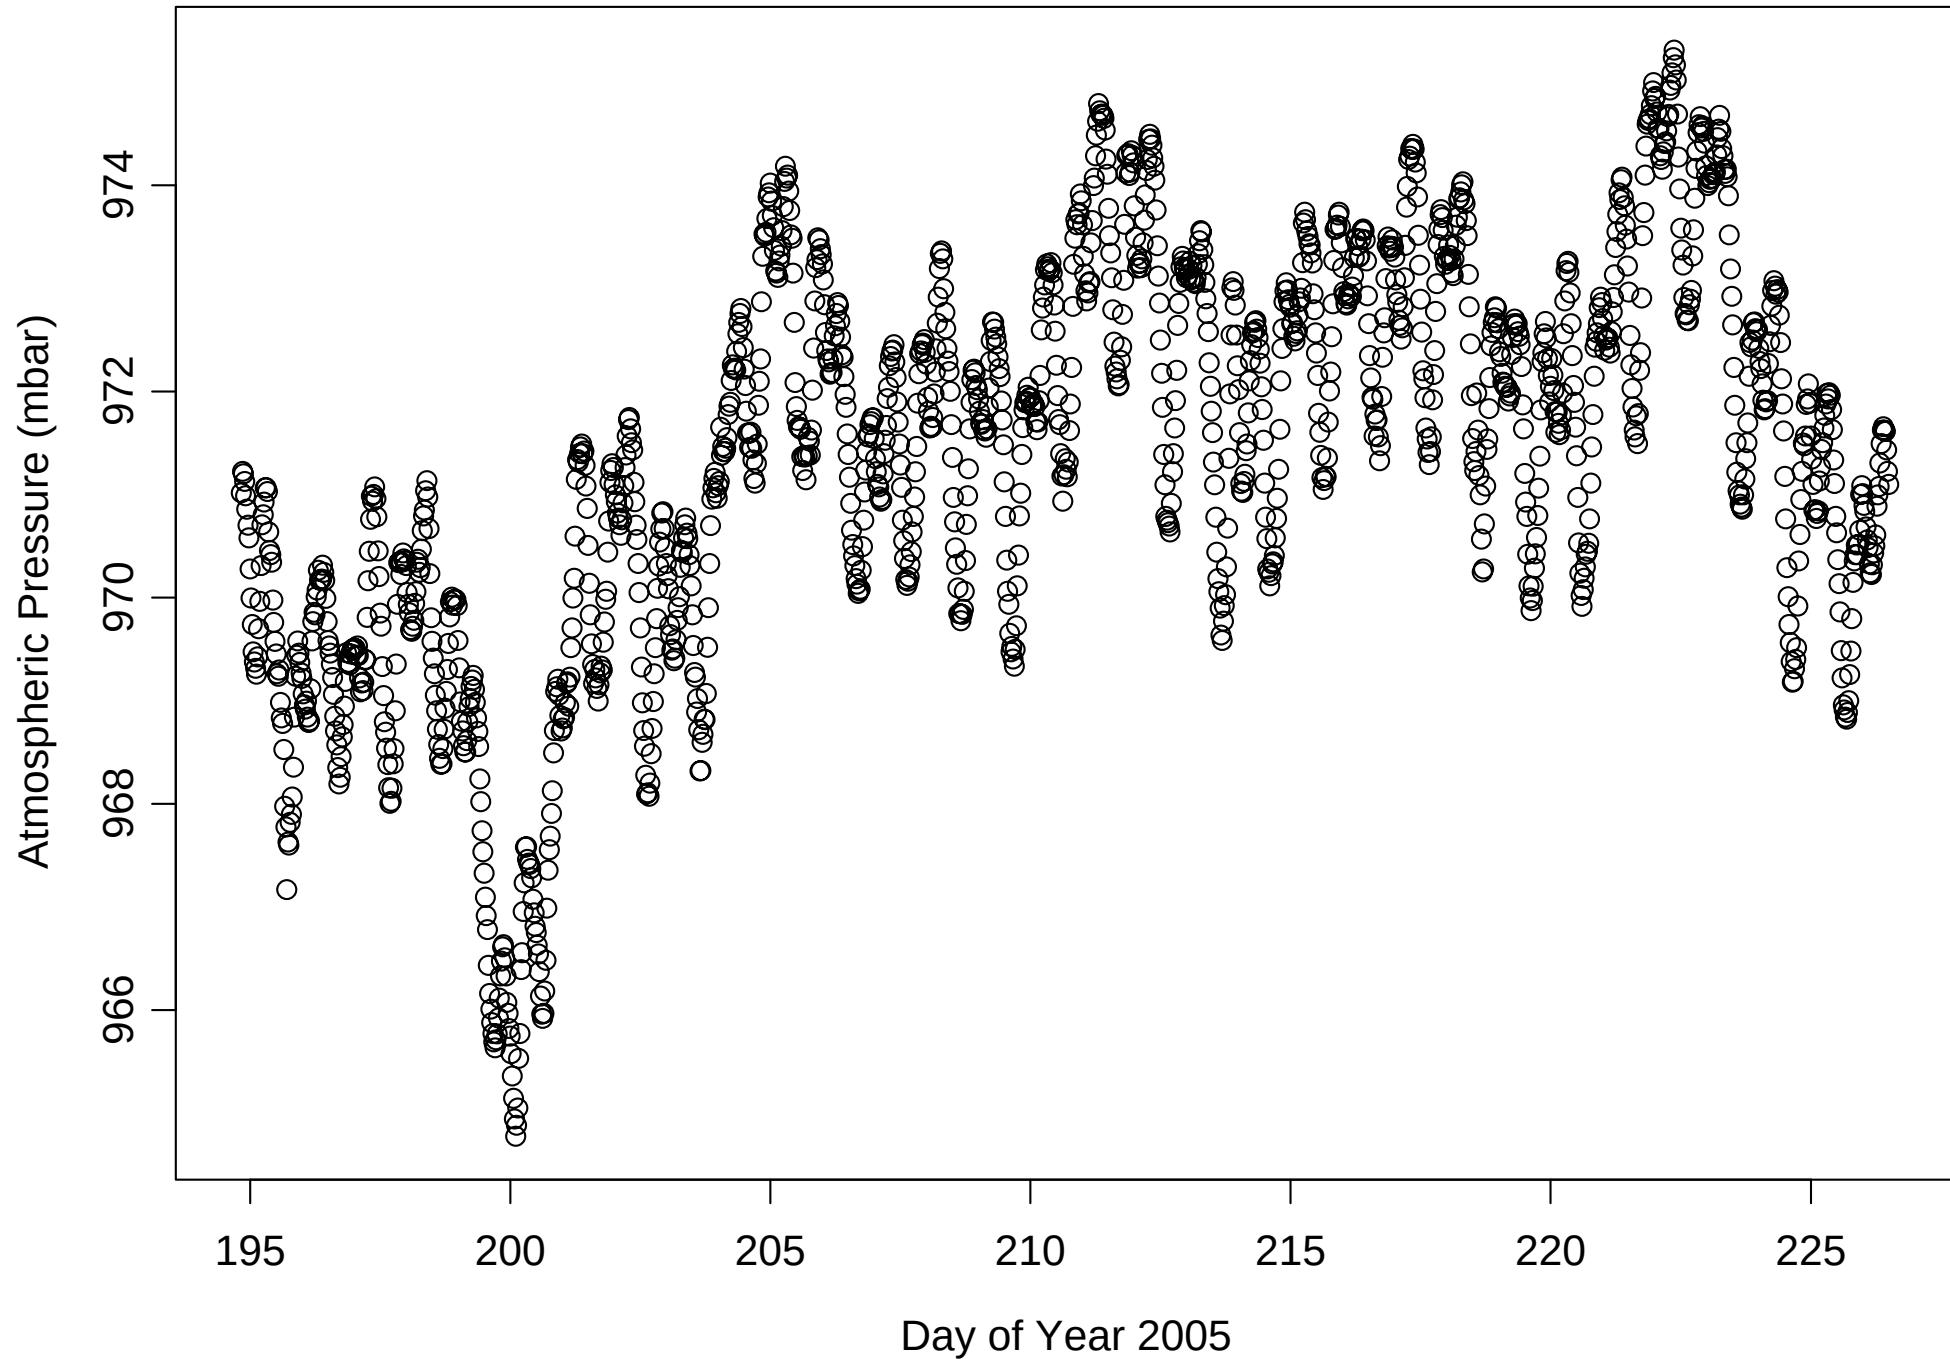


Standard Valve Positions for SDM 5 & 7

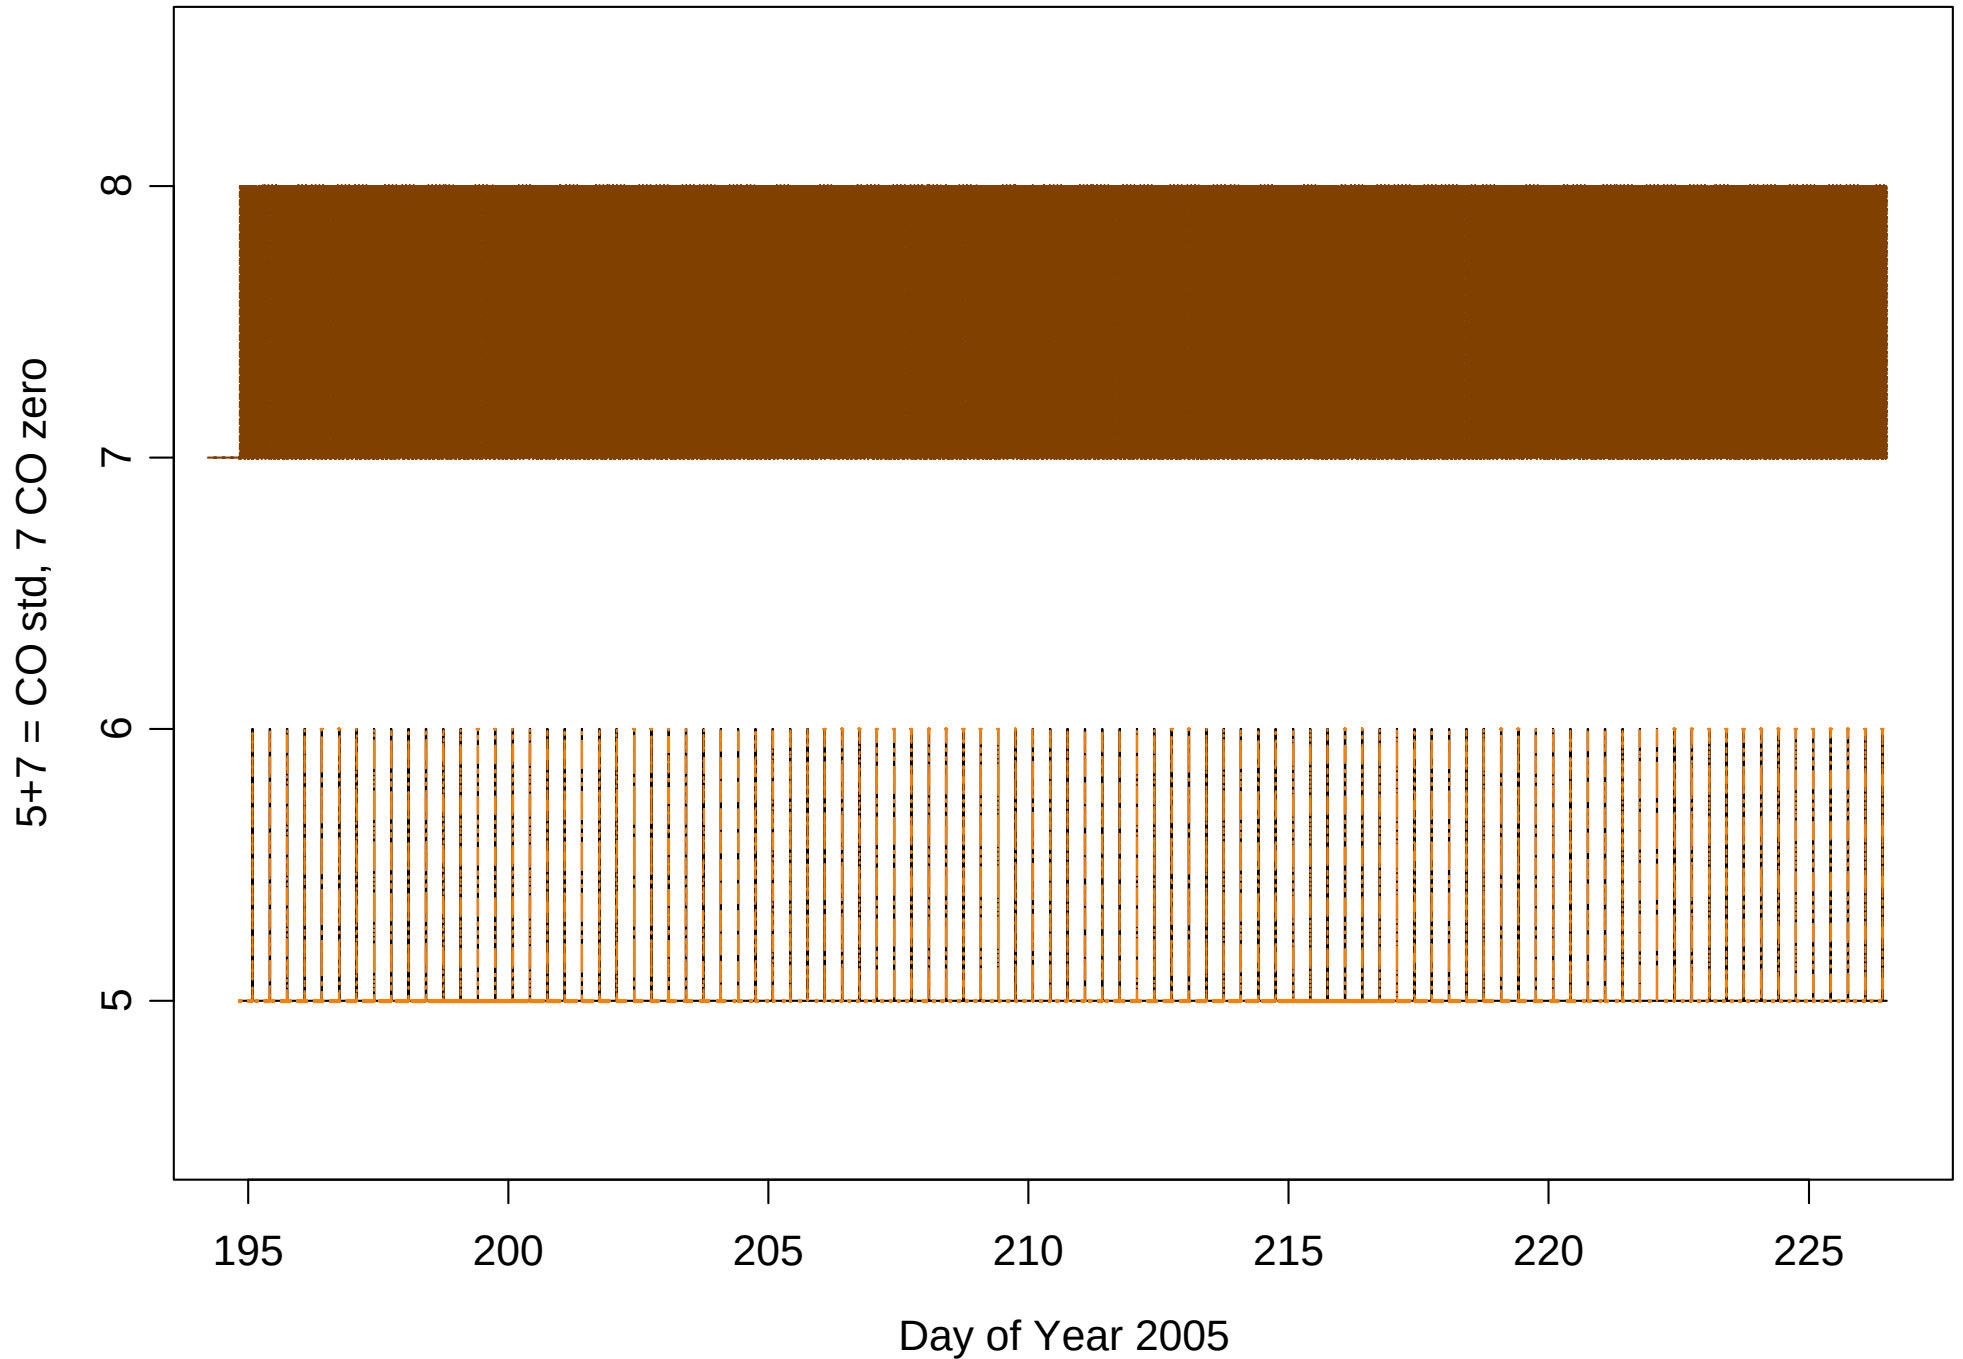


H2O Concentration

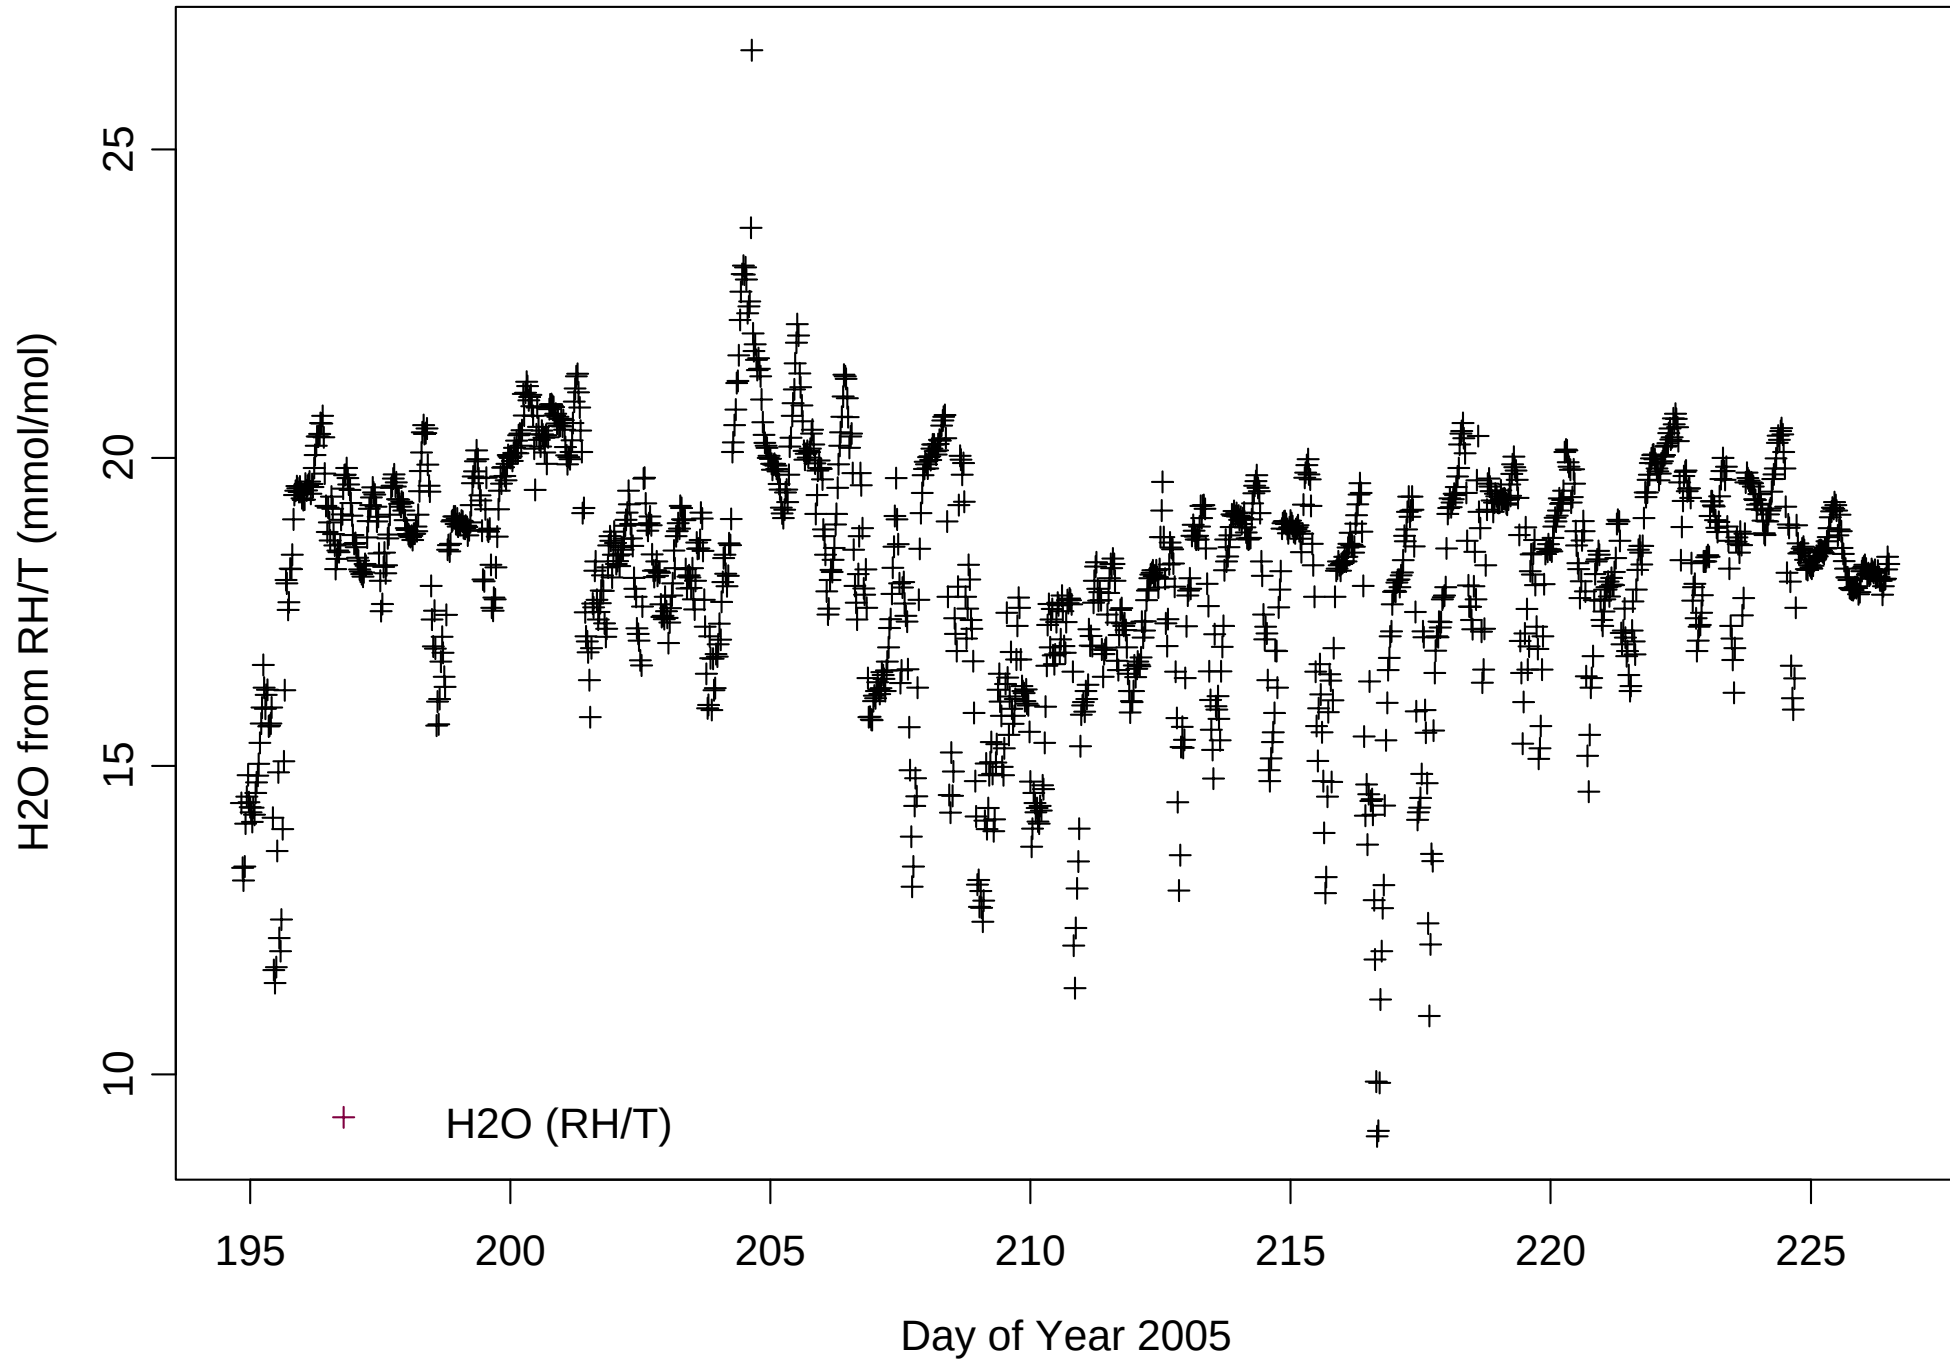


CO Water Trap temp

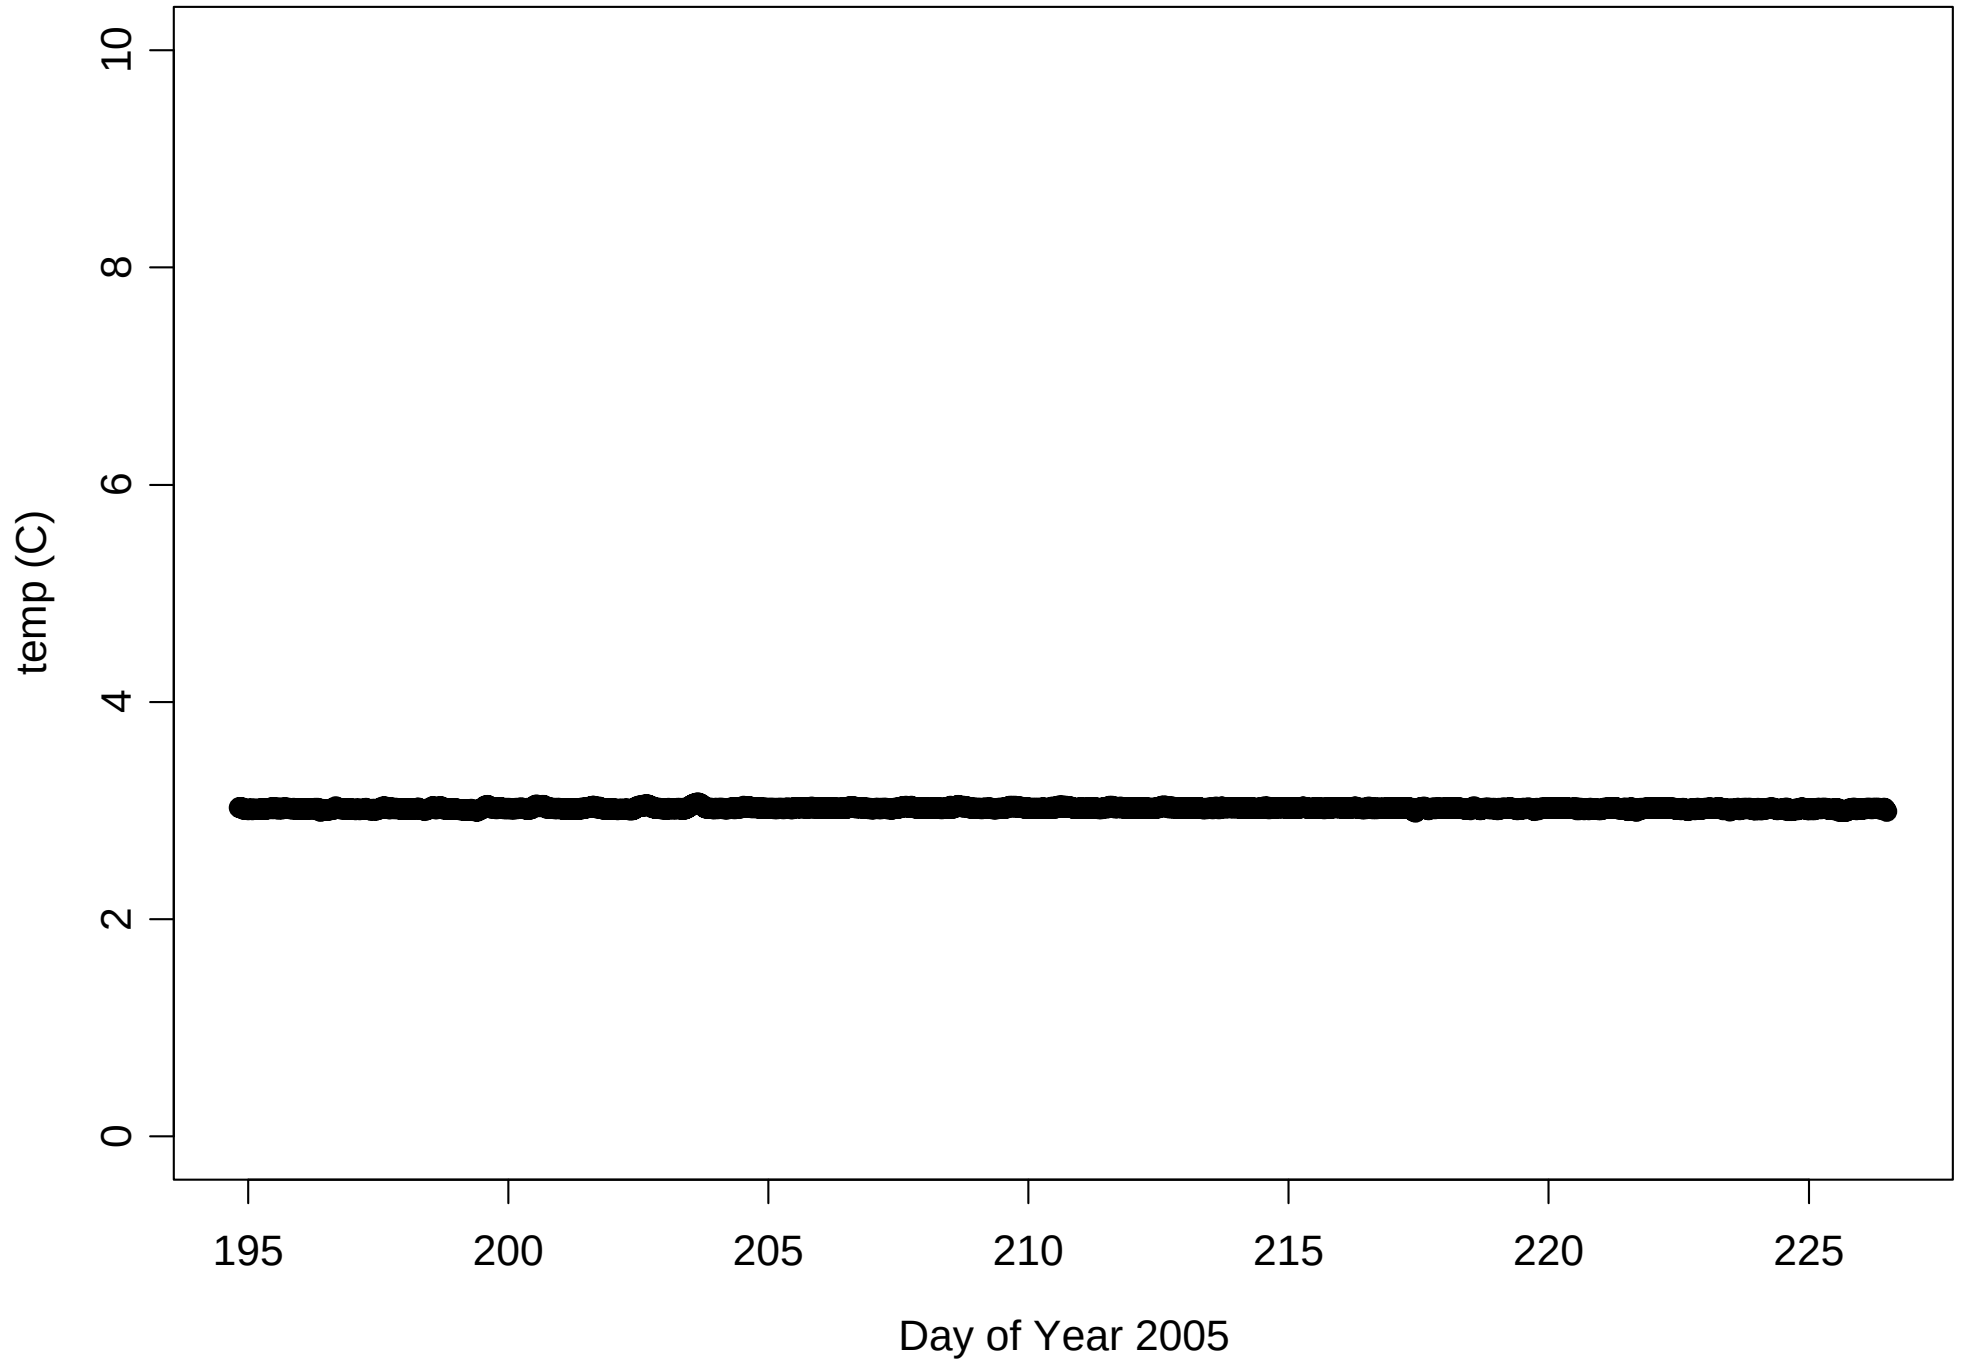


CO Main Flow

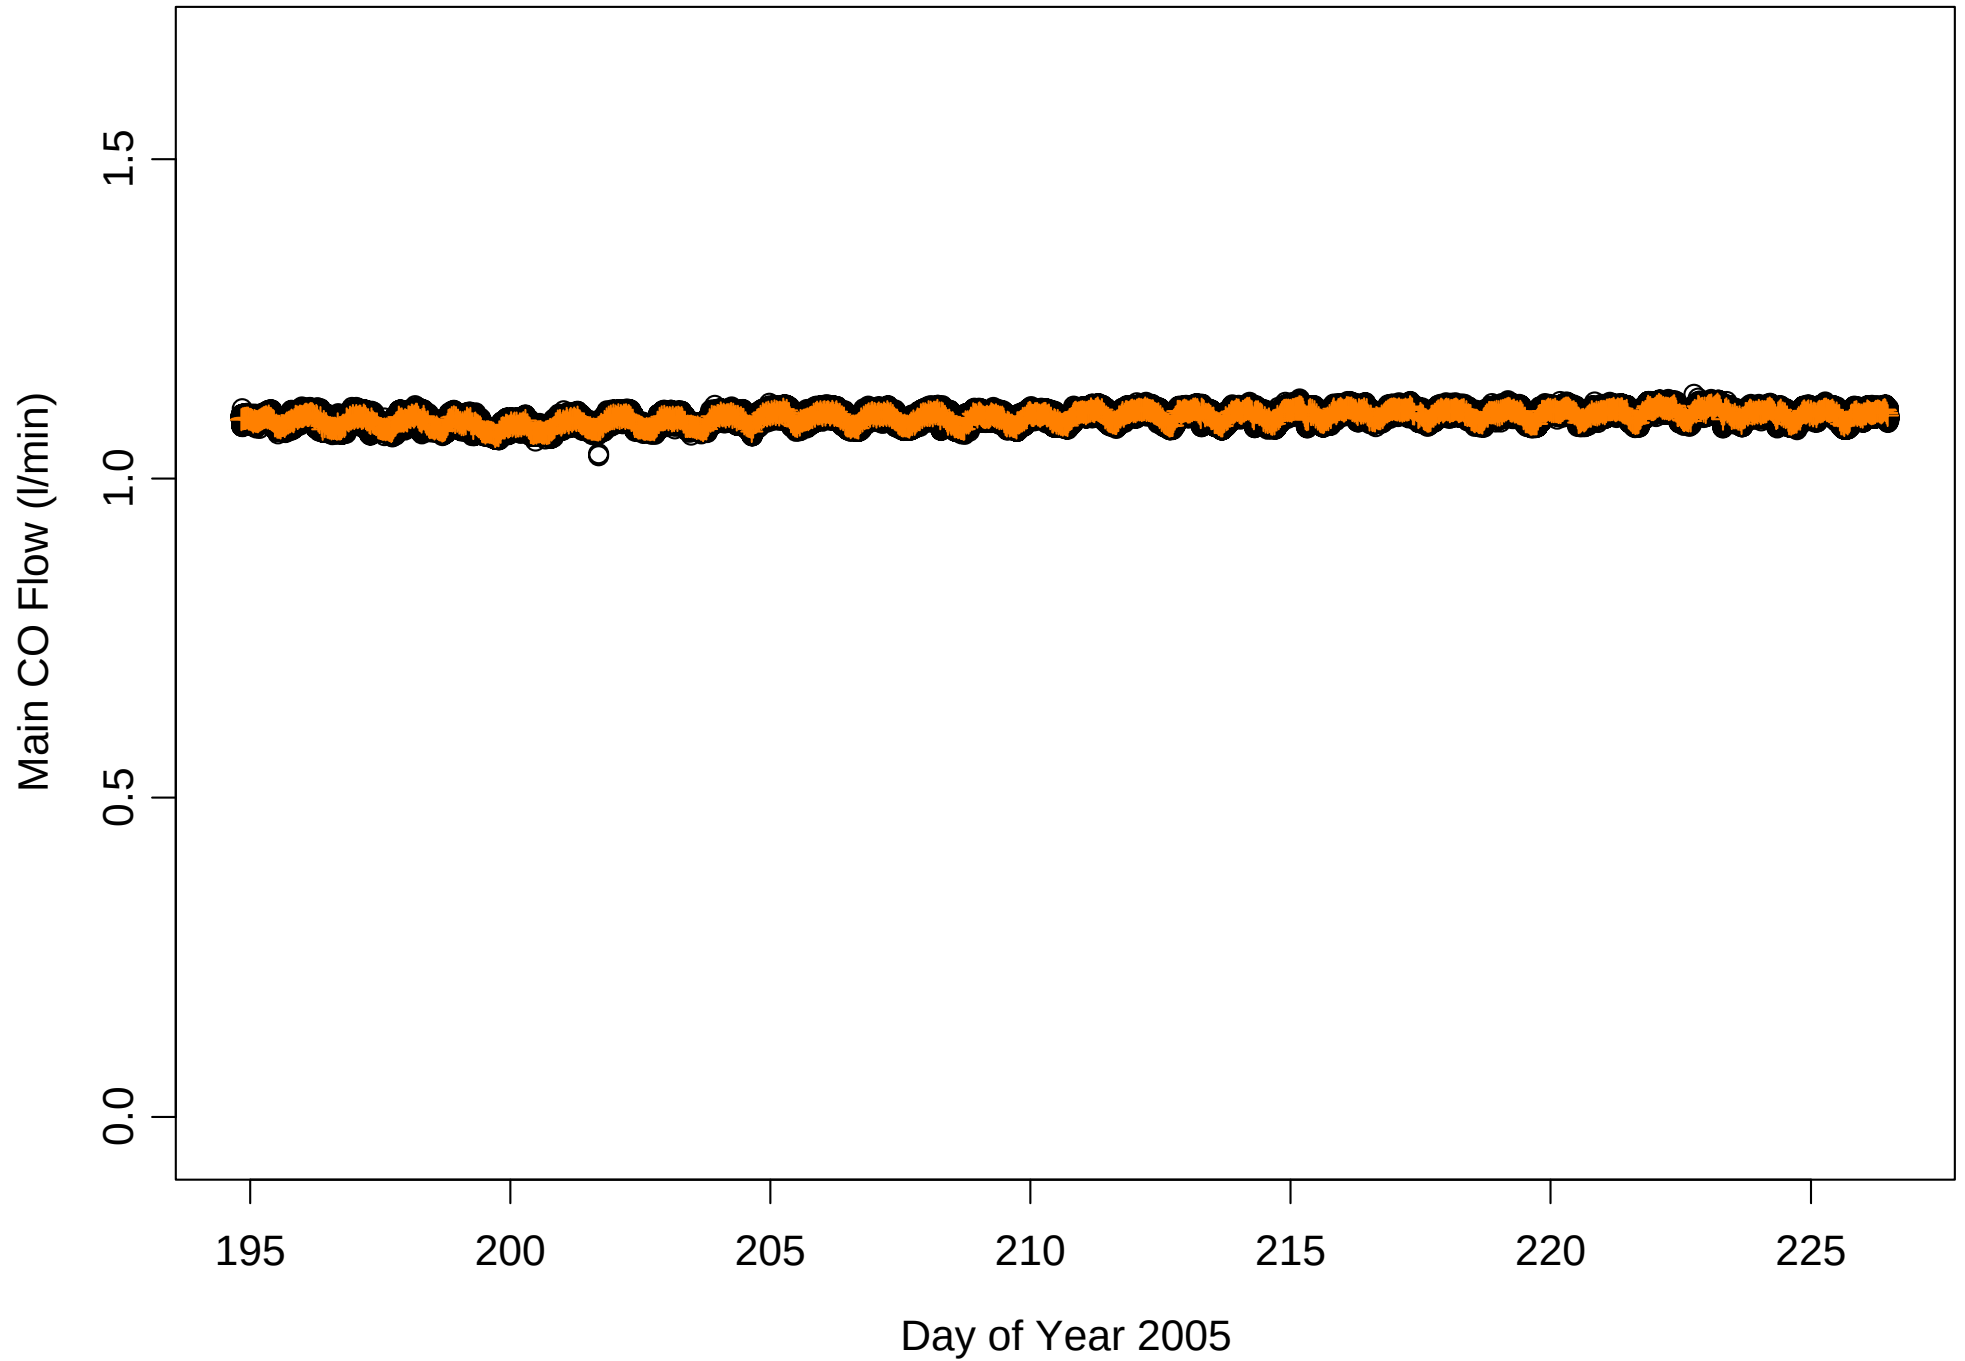


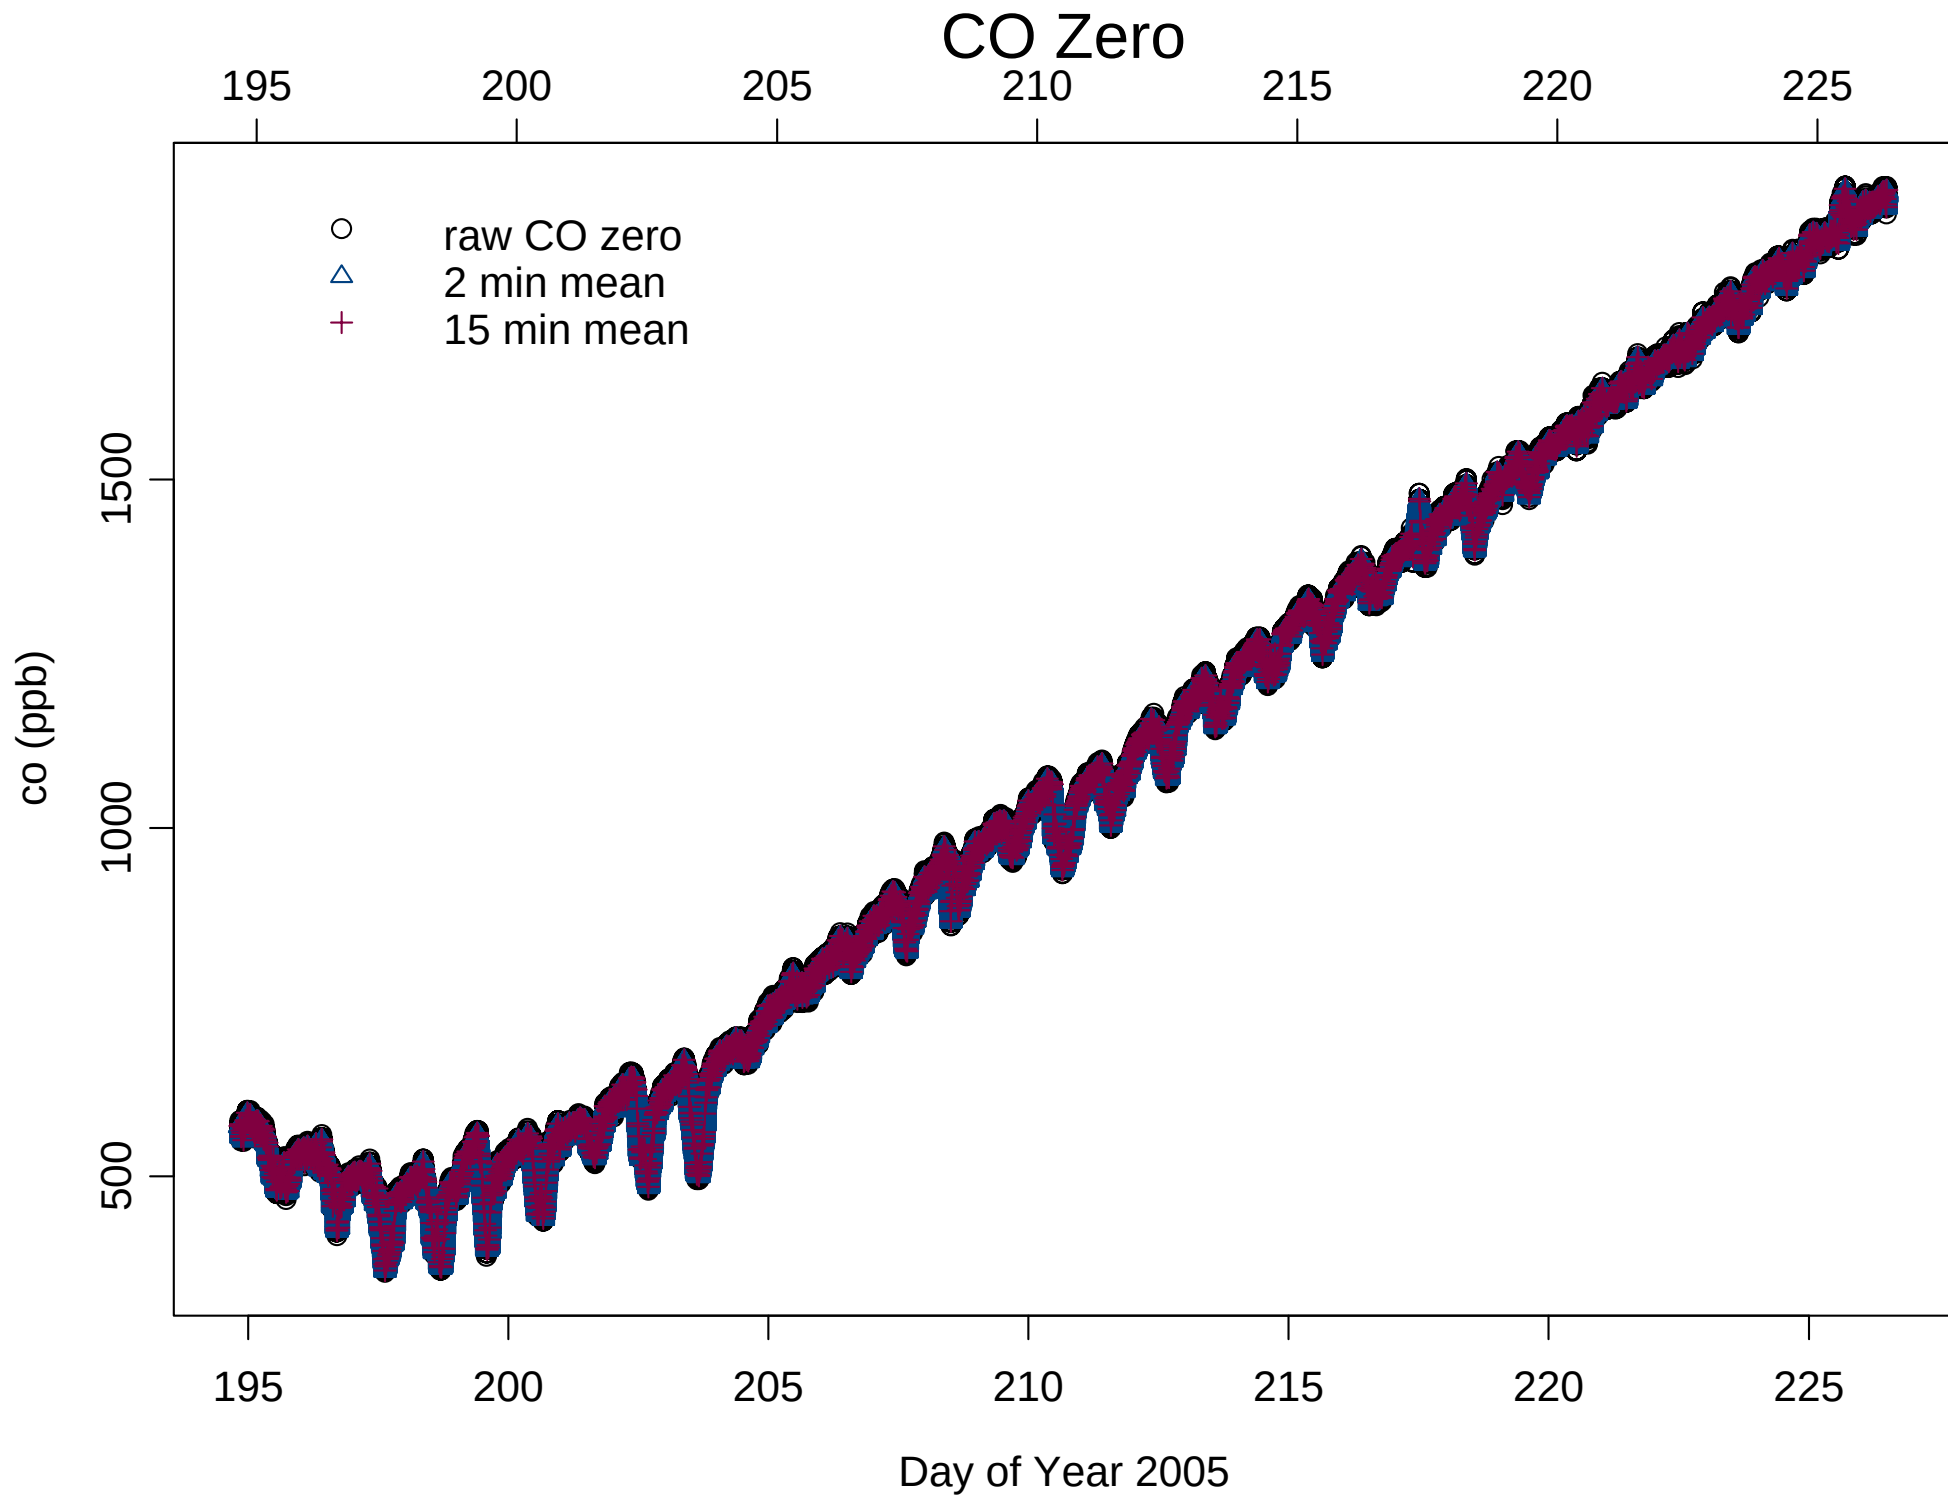


CO Standard Flow

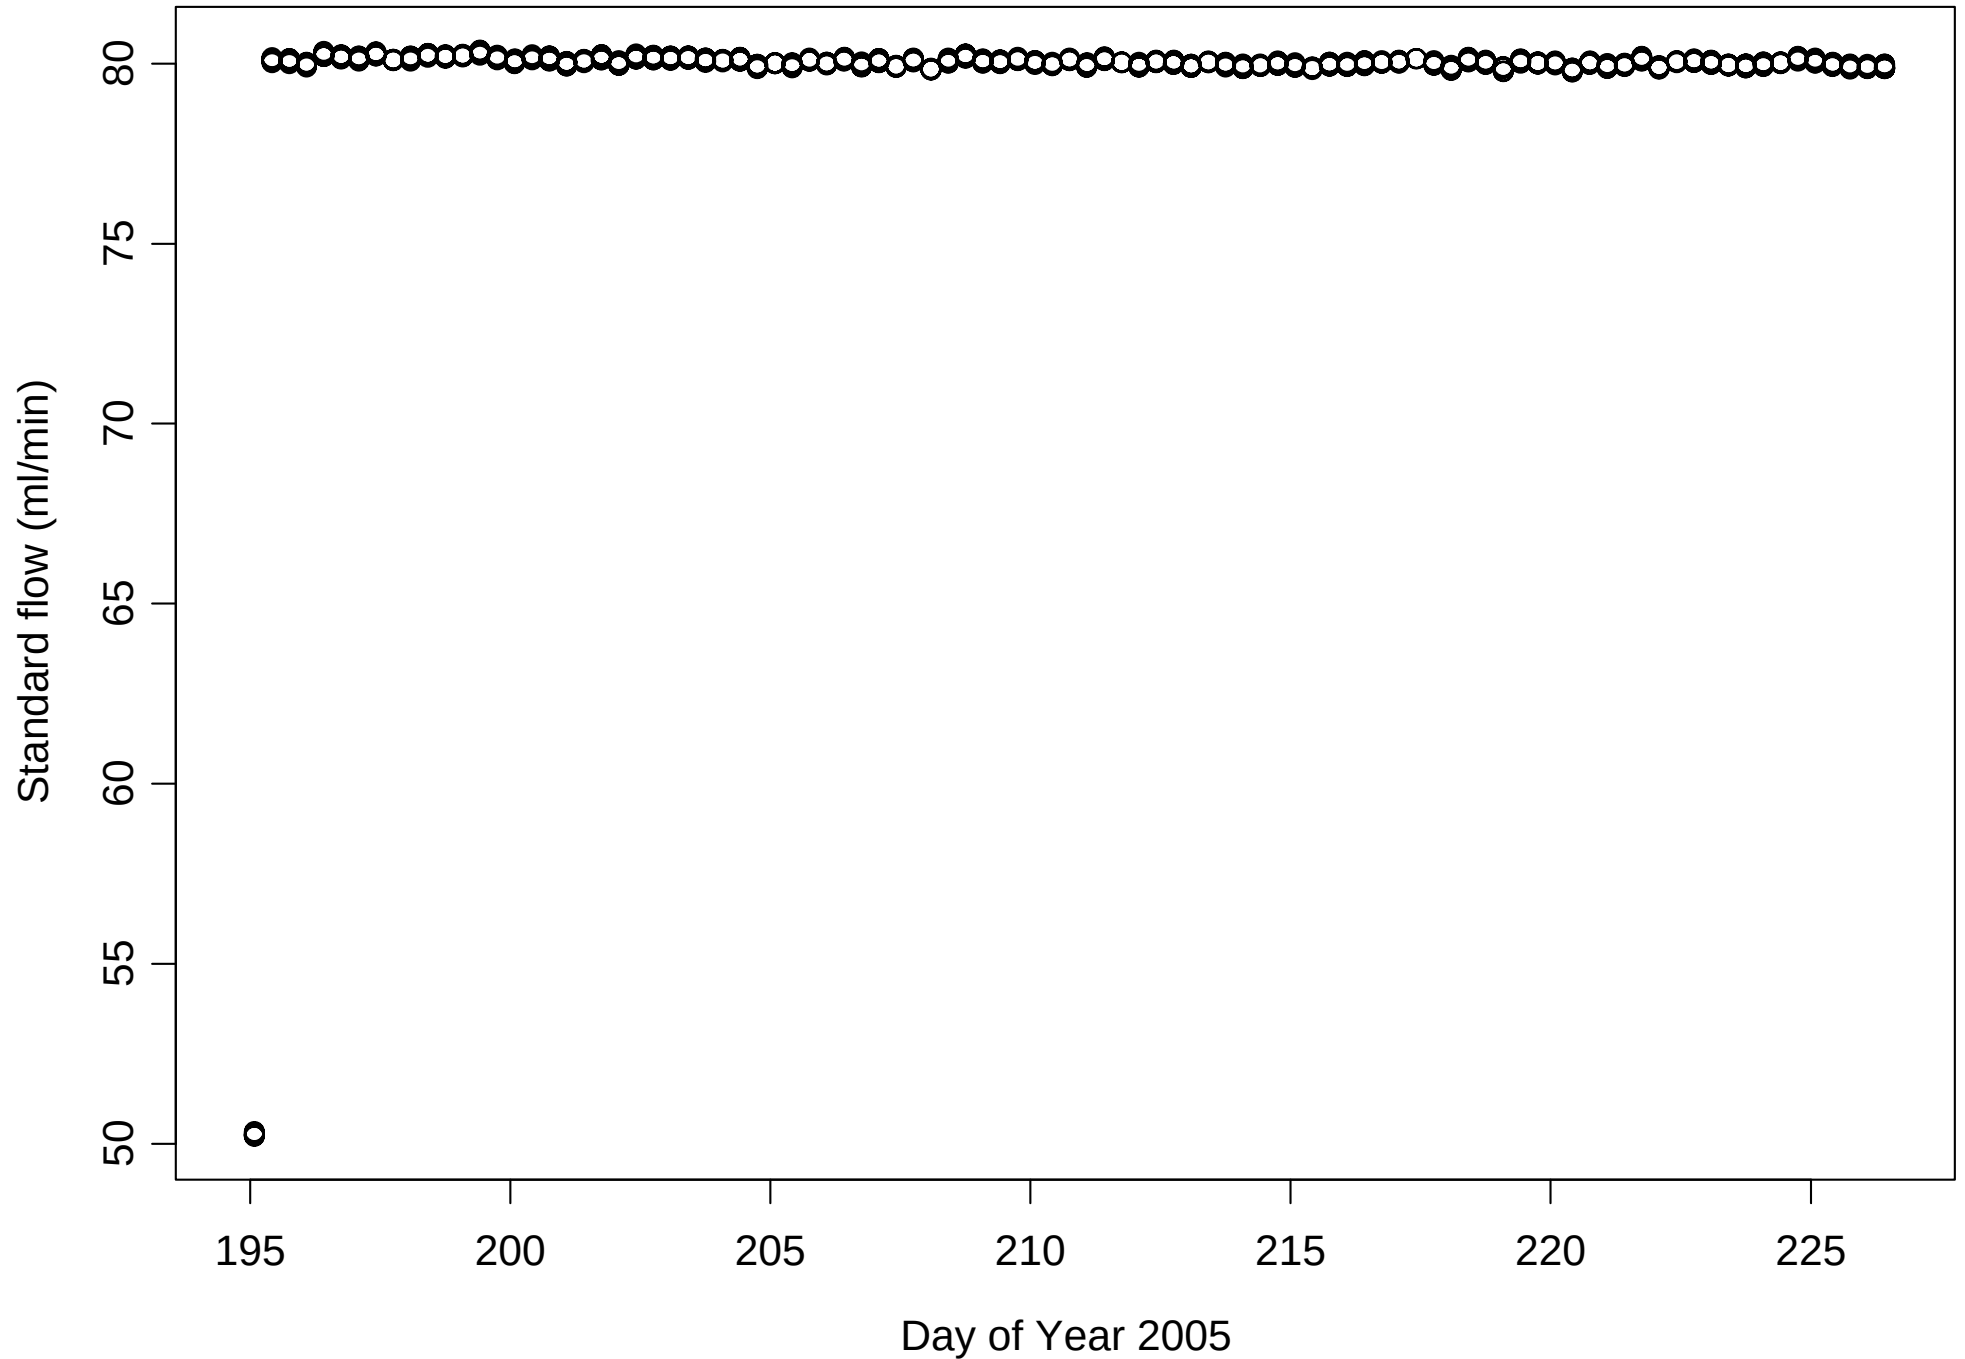

Correction factor for CO cals = 0.965

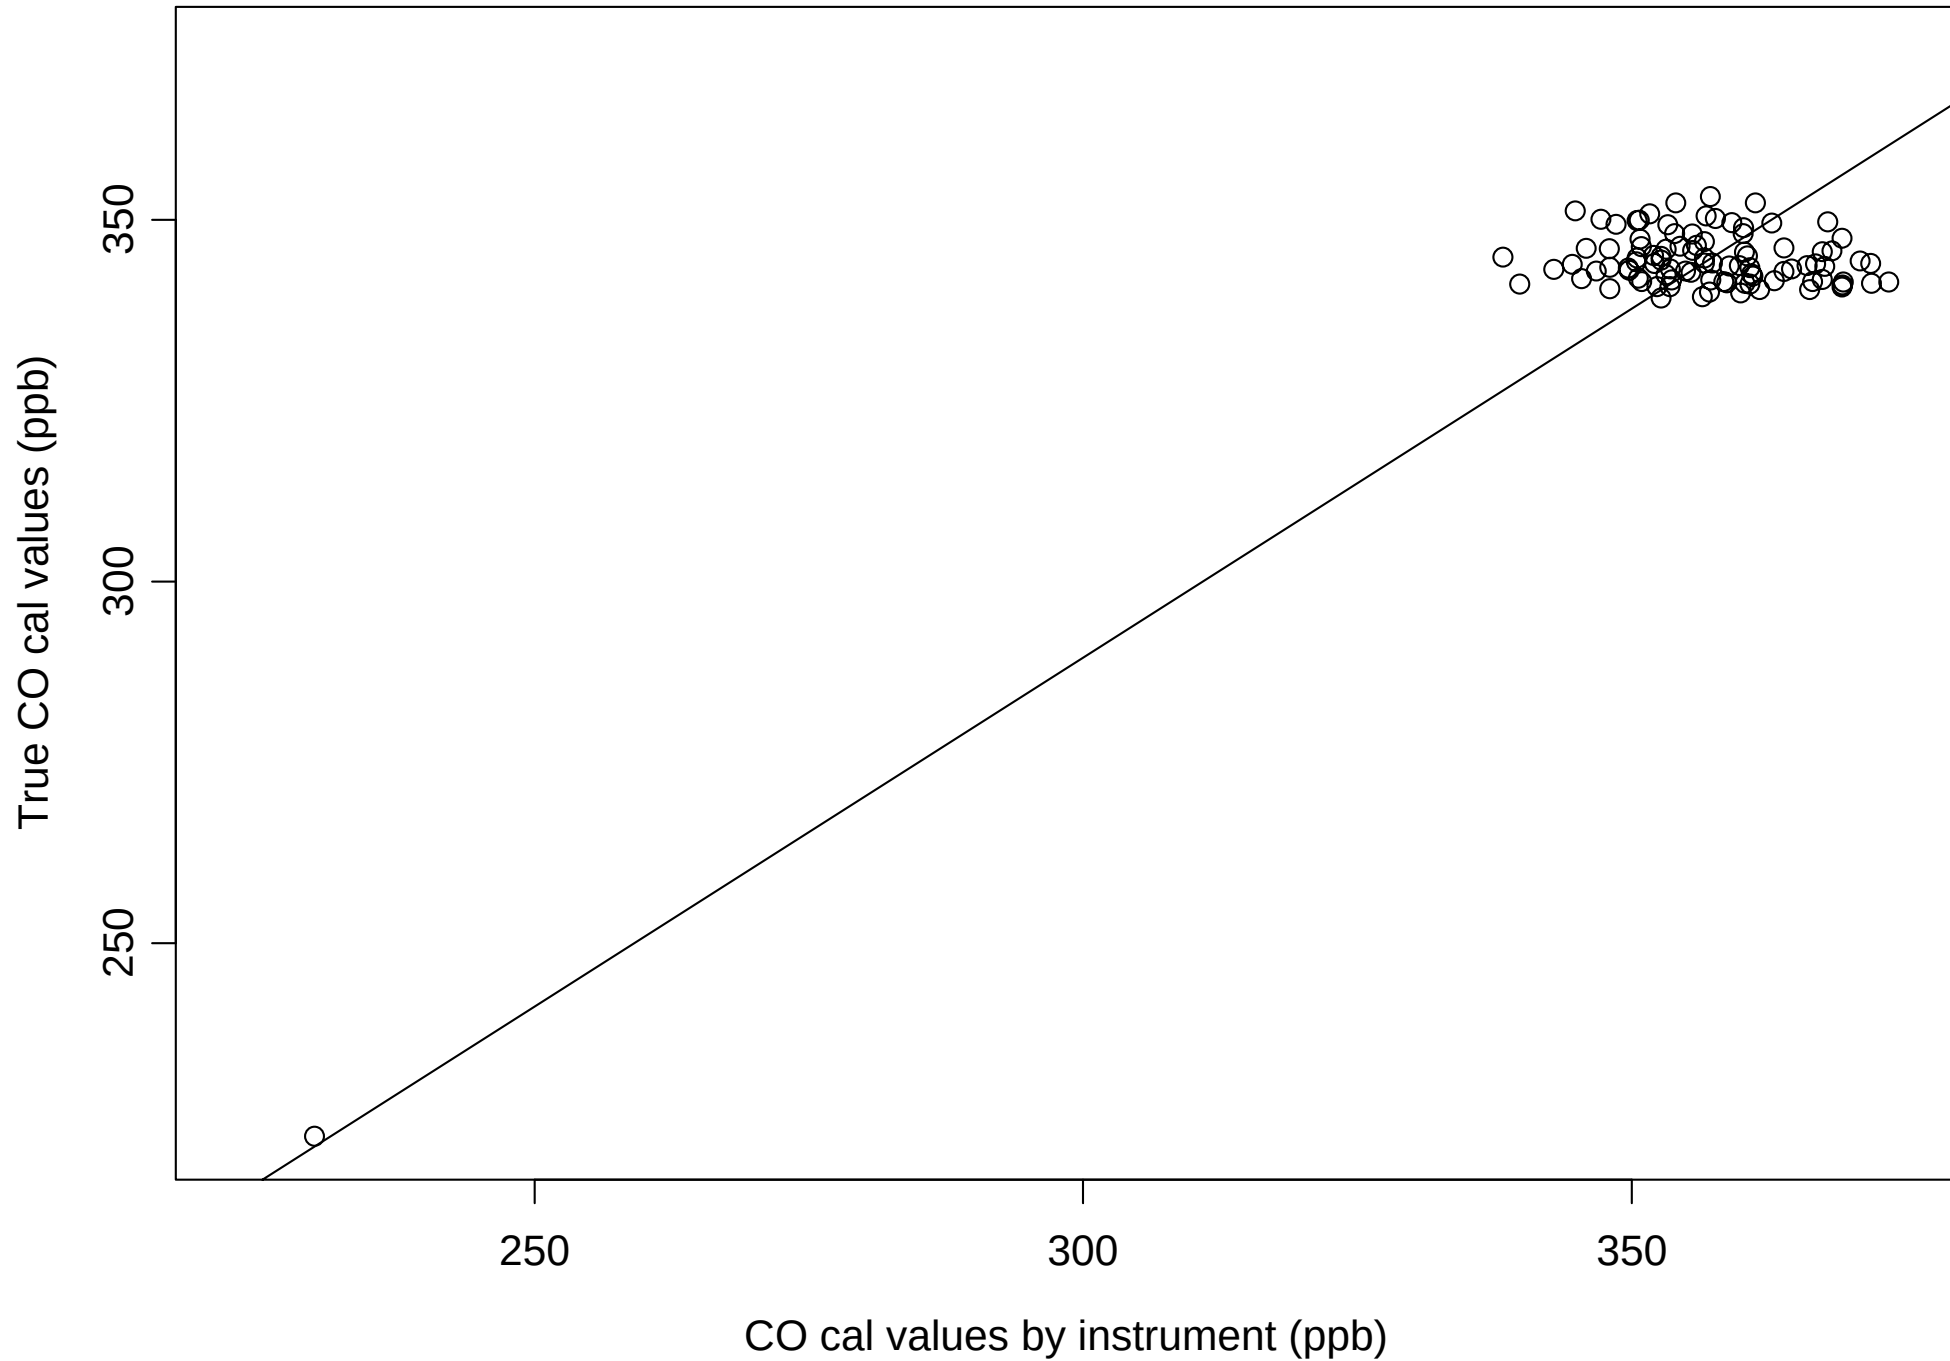

CO minus zero and CO calcs

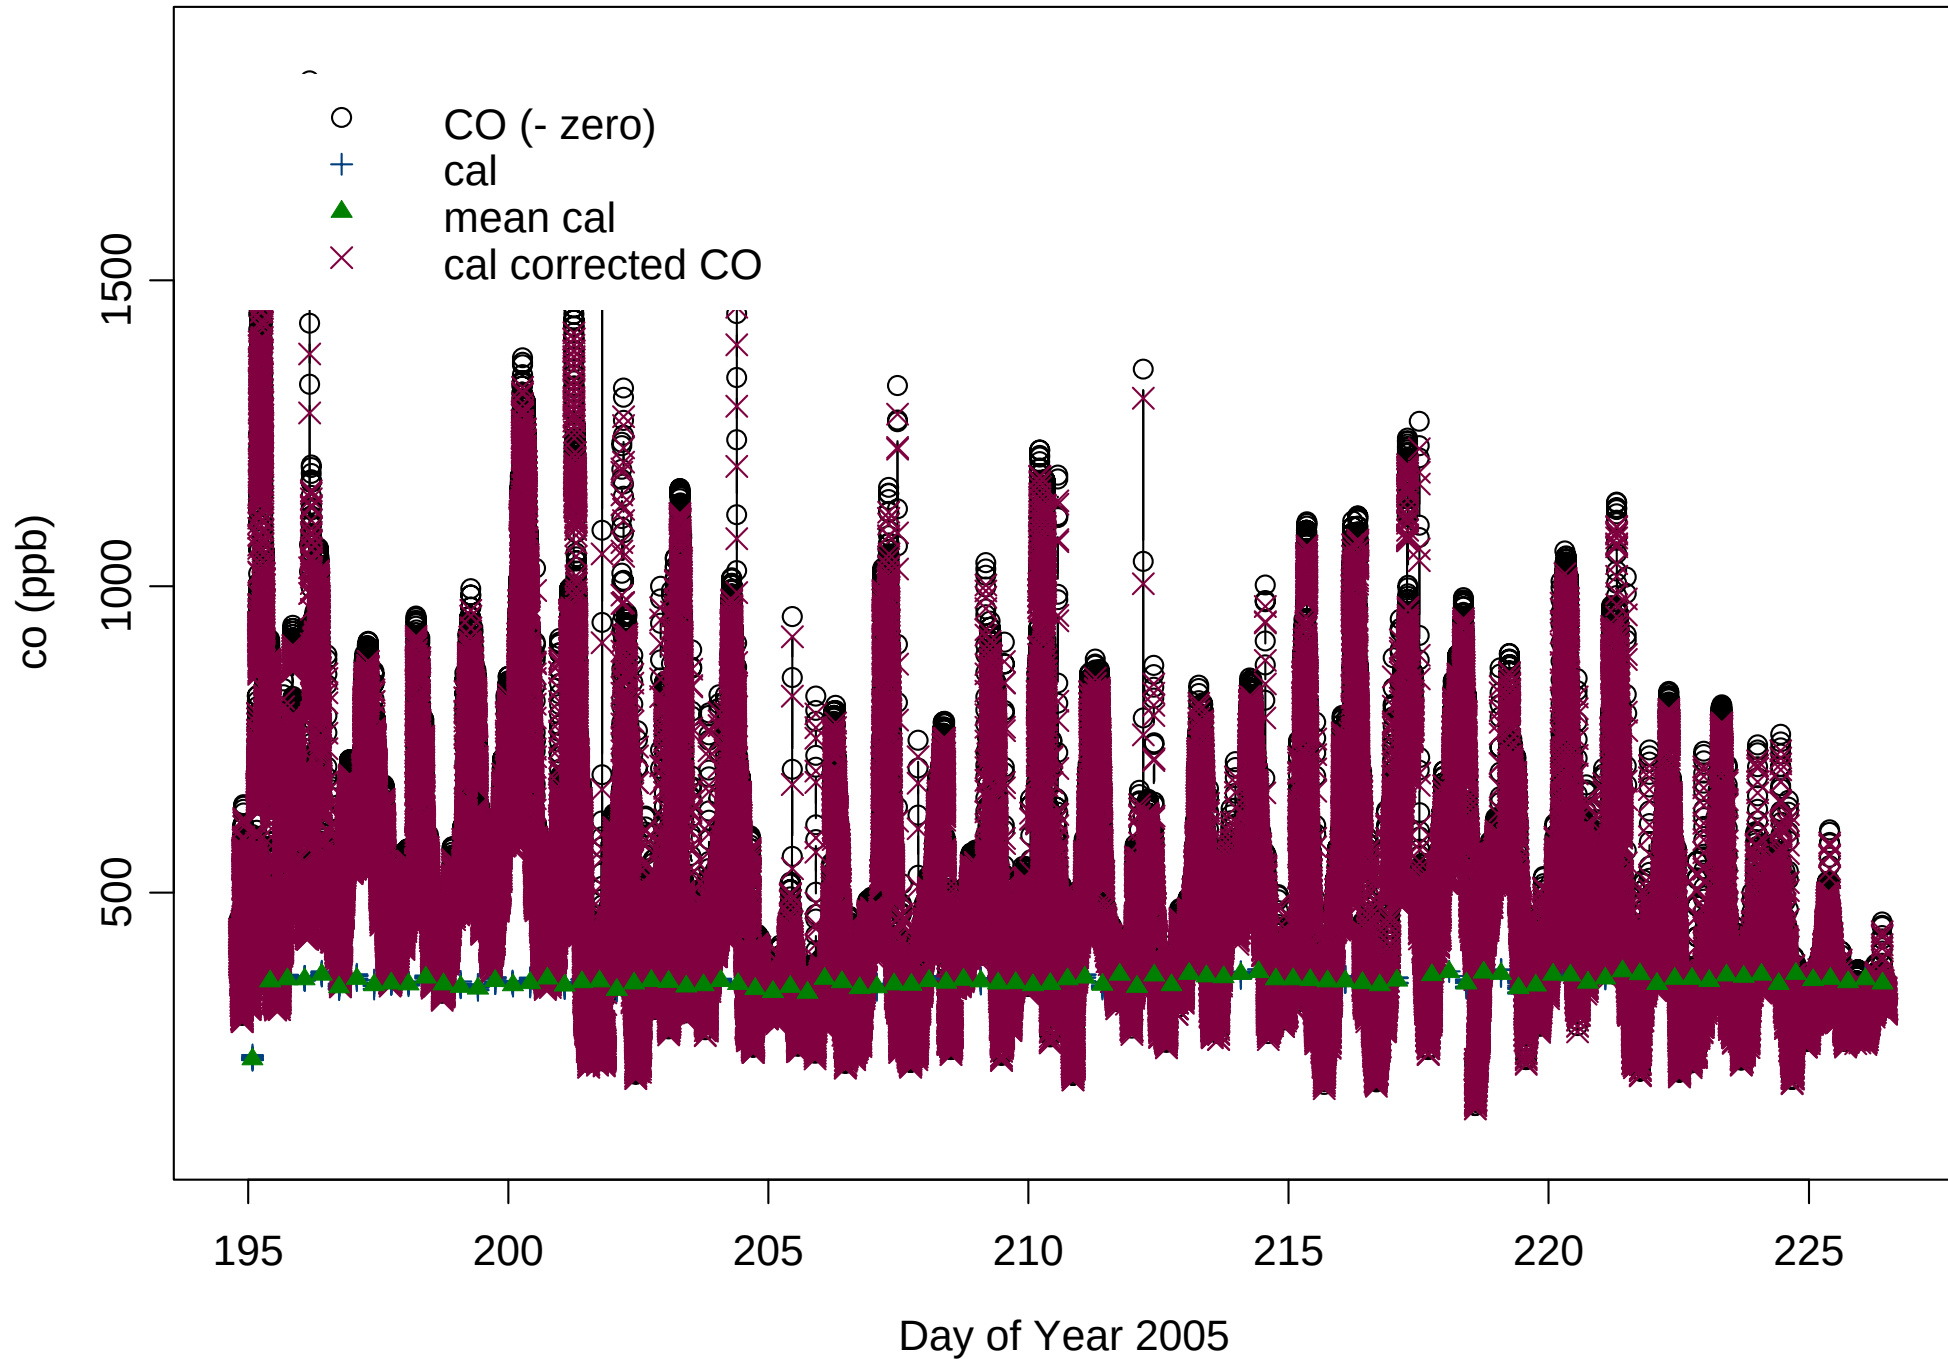

CO Concentration - 30 min values

